



**STATE OF OKLAHOMA  
BOARD OF TESTS FOR ALCOHOL AND DRUG INFLUENCE**

Post Office Box 36307

Oklahoma City, Oklahoma 73136-2307  
Phone: (405) 425-2460 Fax: (405) 425-2490  
www.bot.ok.gov

Dr. Jarrad Wagner, Ph.D. F-ABFT  
Chairman

Joshua Smith  
Director

**ATTESTATION**

I, the undersigned Joshua Smith (Director/Records Custodian), attest under oath pursuant to 12 O.S. §2902 (11)(a) this record was made, at or near the time of the occurrence of the matters set forth by or from information transmitted by a person having knowledge of those matters; was kept in the course of the regularly conducted business activity of the Board; and was made pursuant to the regularly conducted activity. The duplicate record provided is listed below:

- 1) The attached "Service Overview" is a true and accurate copy of maintenance performed on the Intoxilyzer 8000, serial number \_\_\_\_\_, in compliance with the agency's Maintenance Policy and Procedures.

This packet consists of \_\_\_\_\_ pages.

Signed 

Name of Position: Director/Records Custodian

Date of Attestation:

# Service Overview

Board of Tests for Alcohol and Drug Influence  
Enhancing public safety by ensuring the accuracy and scientific reliability  
of blood and breath testing



3600 N. Martin Luther King Bldg #9  
Oklahoma City, OK 73111  
405-425-2460

**BENCH CHECK DATE:** 10-19-2020

**SERIAL:** 80-003395

## **DOCUMENTATION WITHIN SERVICE PACKET:**

- BOT Certificate of Calibration and Operation
- CMI Certificate of Calibration 10-12-2020
- Bench Check
- Bench Check Technician's Report
- BOT Dry Gas Certificate of Analysis
- CMI Service Evaluation Form
- CMI Work Order
- Mock Subject Test
- BOT Certificates of Analysis on Certified Solutions (4)



**STATE OF OKLAHOMA  
BOARD OF TESTS FOR ALCOHOL AND DRUG INFLUENCE**

Administrative Office at:  
Board of Tests for Alcohol and Drug Influence  
Post Office Box 36307  
Oklahoma City, Oklahoma 73136-2307

**Certificate of Calibration and Operation**

This is to certify that the calibration of **INTOXILYZER 8000**, serial number 80-003395, manufactured by CMI Inc., a subsidiary of MPD, Inc. of Owensboro, Kentucky, was tested and found to be in compliance with National Highway Traffic Safety Administration Standard for Devices to Measure Breath Alcohol (F.R., No. 179 48705-48710 Sept. 17, 1993) and with International Recommendation OIML R 126 Edition 1998 (E). Calibration solutions are traceable to NIST standard material 1828.

In addition the operational procedures and functions of this Intoxilyzer have also been tested and found to be in compliance with the Oklahoma Board of Tests for Alcohol and Drug Influence - Rules and Regulations OAC Title 40: 25-1-2 and 30-1-3 and is hereby certified for use as an evidential breath testing device within this state.

CERTIFICATION TYPE	DATE
Manufacturer Calibration	08-27-08
Board of Tests Bench Check	11-13-08
Manufacturer Calibration	10-18-11
Board of Tests Bench Check	10-26-11
Board of Tests Bench Check	03-23-10
Board of Tests Bench Check	09-09-13
Board of Tests Bench Check	05-11-15
Board of Tests Bench Check	01-22-16
Board of Tests Bench Check	11-08-16
Board of Tests Bench Check	09-11-18
Board of Tests Bench Check	07-15-20
Manufacturer Calibration	10-12-20
Board of Tests Bench Check	10-19-20



Presentation of this form certifies that the Intoxilyzer, SN: 80-003395, functioned properly at the time of the breath test and hereby certifies the breath test result as valid.

Date:

Re: Request for Log of Test on Intoxilyzer 8000

Name:

Dear Sir:

The Log of Test information from a breath test conducted on a Intoxilyzer 8000 is printed in Section 2 of the Affidavit and is no longer retained as a separate form as with the Intoxilyzer 5000. The 8000 uses a nitrogen/ethanol dry gas for the external control test. The dry gas cylinder has the capacity to perform approximately 325 tests and does not require maintenance until its expiration date or can no longer provide the required pressure to perform a control test. The cylinder has an expiration date of two years from date filled at the manufacturer and is programmed in the 8000 upon installation, both dates are printed in Section 2 of the Affidavit. The Intoxilyzer is programmed to disable itself when the date of expiration is reached or the pressure monitor indicates 25 lbs psi.

Due to the reliability and stability of dry gas, maintenance on the 8000 is not required every 30 days or 25 tests, therefore maintenance is no longer performed by officers in the field. The Board of Tests for Alcohol and Drug Influence certifies each Intoxilyzer 8000 for field use by performing a bench check. The bench check is designed to check the operation and procedures programmed in the 8000 to ensure it is functioning properly for use in Oklahoma. A bench check is performed every time a new dry gas cylinder is installed or the instrument has returned from the manufacturer for repair. Once the instrument passes the bench check, all that is required to set it up for field use is to plug it in and turn it on and does not require a permit to set up. The Board of Tests has the ability to monitor each instrument once it is set up in the field.

Each Intoxilyzer has a database of valid permit numbers that it checks prior to allowing a breath test to be performed. The database is updated on a regular basis, if a permit number is invalid that officer will not be able to conduct a breath test on the 8000. If the 8000 prints an affidavit the breath test operator listed in Section 2 had a valid permit at the time of the test and the breath test is valid.

If you have any further questions please feel free to call me.

Sincerely,



J. Robert Blakeburn (OBA11059)  
State Director of Tests for Alcohol  
and Drug Influence



# Certificate of Calibration

This is to certify the calibration of **Intoxilyzer**® serial number 80-003395, manufactured by CMI Inc., a subsidiary of MPD, Inc. of Owensboro, Kentucky, was tested and found to conform to the National Highway Traffic Safety Administration (NHTSA) Standard for Devices to Measure Breath Alcohol (Federal Register, Vol.58, No.179, pp 48705-48710, Sept. 17, 1993) for accuracy and precision. Reference materials are traceable through the National Institute of Standards and Technology (NIST) to the International System of Units (SI).

Date Oct 12, 2020

Signed

Alice Loler

Technician

**EMI** INC.

316 East 9<sup>th</sup> Street  
Owensboro, KY 42303  
USA

Part No. 650517 Rev.A

**STATE OF OKLAHOMA - BOARD OF TESTS FOR ALCOHOL AND DRUG INFLUENCE  
CMI INTOXILYZER BENCH CHECK PROCEDURE REPORT**

BENCH CHECK DATE 10/19/2020	TIME PROCEDURE BEGAN 11:10:4	INSTRUMENT LOCATION 80-003395
INSTRUMENT TYPE Intoxilyzer	INSTRUMENT MODEL I-8000	INSTRUMENT SERIAL NUMBER 80-003395

**TEST RESULTS**

**Diagnostics**

PASS

**Mouth Alcohol Test**

PASS

**RFI Test**

PASS

**Abort Test**

PASS

**Improper Sample Test**

PASS

**Interferent Detect Test**

PASS

**No Sample Given Test**

PASS

**Insufficient Sample Test**

PASS

**Air Blank Contamination Test**

PASS

**Range Exceeded Test**

PASS

**Duplicate Breath Sampling Results**

Value	Test 1	Test 2	Control Test
.02	0.019	0.018	0.019
.04	0.037	0.036	0.037
.10	0.101	0.100	0.100
.20	0.202	0.199	0.199


PASS

**CERTIFYING TECHNICIAN**

I swear under penalty of perjury that in regards to the above listed instrument, I have complied with the Intoxilyzer Bench Checking Procedure approved by the State of Oklahoma.

SIGNATURE  23020	DATE 10/19/2020
NAME PAPE, CHRISTOPHER	PERMIT # 0000023020





3600 N. Martin Luther King Bldg #9  
 Oklahoma City, OK 73111  
 405-425-2460

# BENCH CHECK TECHNICIAN'S REPORT

**Date:** 10/19/2020

**Start Time:** 11:10

**End Time:** 12:00

**INSTRUMENT**

Intoxilyzer Model	Serial #
8000	80-003395

**GAS CANISTER**

LOT #	EXP Date
22620080A2-009	10/05/2022

**REFERENCE**

Simulator Model			
Guth 2100	Guth 2100	Guth 2100	Guth 2100
Serial #			
DR2834	DR3700	DR2455	DR3470
Concentration			
.02	.04	.10	.20
LOT #			
20070	20060	20190	20160
Manufactured Date			
02/13/2020	02/10/2020	04/06/2020	03/18/2020
Expiration Date			
02/13/2022	02/10/2022	04/06/2022	03/18/2022
Solution Commission Date			
9/28/2020	9/28/2020	10/14/2020	10/14/2020

**REASON FOR BENCH CHECK**

- POST REPAIR     CYLINDER REPLACEMENT
- TROUBLESHOOTING     ROUTINE MAINTENANCE

**COMMENTS**

Modem failed during initial diagnostic after power up.

*Christopher Pape* 23020  
 Technician Signature / Permit #

Christopher Pape #23020  
 Printed Name

Certificate of Analysis – Dry Gas	
9/24/2020	0.080
Date of Analysis	Labelled target value (g/210L)
009	0.078
Cylinder #	Average test result
Christopher Pope <i>Christopher Pope</i> 23020	
BOT Technician Name and Signature	



8/16

ALPHA INSTRUMENT 2  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-004923  
09/24/2020 10:02

In accordance with BOT Policy and Procedure Statement BRT-2.3.0, Maintenance, the above referenced dry gas cylinder is suitable for use as an external reference with the Intoxilyzer 8000.  
7 Eastgate Dr. • P.O. Box 790 • Jacksonville, IL 62651-0790  
217-245-2183 • Fax: 217-243-7634 • www.ilmoproducts.com

Test	g/210L	Time
Air Blank	0.000	10:03
Cal Check	0.078	10:03
Air Blank	0.000	10:04
Cal Check	0.078	10:04
Air Blank	0.000	10:04
Cal Check	0.078	10:05
Air Blank	0.000	10:05
Cal Check	0.078	10:06
Air Blank	0.000	10:06
Cal Check	0.078	10:06
Air Blank	0.000	10:07
Cal Check	0.079	10:07
Air Blank	0.000	10:08
Cal Check	0.078	10:08
Air Blank	0.000	10:09
Cal Check	0.078	10:09
Air Blank	0.000	10:09
Cal Check	0.078	10:10
Air Blank	0.000	10:10
Cal Check	0.079	10:11
Air Blank	0.000	10:11
Cal Check Stats		
Average	0.0782	
Std Dev	0.0004	
Rel Std Dev(%)	0.5391	

## Certificate of Analysis

Certificate ID: 13253 ✓  
Part #: BAC105L080T  
Cylinder Size: 105L  
Lot Number: 22620080A2 ✓  
Expiration: 10/5/2022 ✓

*RCV'D  
9/22/2020  
CP*

0.080 BAC (For the calibration of instruments used to determine breath alcohol concentration)

Contents: 105 Liters @ 1000 psig 70°F (21°C)

Component:	Reported Concentration:	Analytical Accuracy (U, k=2):	Analytical Method:
Ethanol	208 ppm	+/-0.002 BAC(G/210L)	NDIR
Nitrogen	Balance	[5.2 ppm]	

**Distributed by:**

CMI Inc.  
316 East Ninth Street  
Owensboro, KY 42301  
Phone 866-835-0690  
[www.alcoholtest.com](http://www.alcoholtest.com)

*Christopher Pope*  
Operator's Signature

\*Traceable to:  
Certified Reference Material - 262.4 µmol/mol  
Ethanol in Nitrogen - Serial No. GN0015026 Lot No. 050319E11

Store in dry area, away from sources of heat, ignition and direct sunlight. Do not allow storage area to exceed 52 °C (125 °F).

*Joshua...*  
Specialty Gas Lab Tech  
*Travis...*

09-03-2020  
Issuance Date



The calibration results within this certificate were obtained using equipment and standards capable of producing analytical results traceable to NIST, and apply only to the items contained on this certificate. ILMO Products Company makes no warranty or representation as to the suitability of the use of any information provided for any particular purpose. The information use is at the sole discretion and risk of the user. Liability shall be limited to established replacement cost of this material or service.



# CMI INC. Service Evaluation Form

This form **MUST** be completed and enclosed with instrument to be serviced.  
Failure to complete and return this form may cause delays in service.

(Note: please ship items in their original shipping container(s) or a similar protective box.)

1. Contact information: Customer Number **731362** (contact Customer Service)  
Name: **Board of Tests** Phone: **(405) 425 2460**  
Fax: **(405) 425 2490** Email: **christopher.pape@bot.ok.gov**

2. Bill to Address: **Board of Tests** Ship to Address: **Board of Tests**  
**3600 N ML King, Bldg 9** **3600 N ML King, Bldg 9**  
**OKC, OK 73111** **OKC, OK 73111**

3. Serial Number: **80-003395** Instrument Model: **Intoxilyzer 500 / 8000**


4. Detailed Description of Problem:  
**Diagnostic fail on modem. Modem replaced. Unit still gives diagnostic fail on modem.**

\*\*\*Hazardous Material Warning! - DO NOT return gas cylinders with instrument!\*\*\*

I Authorize Repairs Up To:  All  \$250  \$500  \$750  Other \$ \_\_\_\_\_  
Purchase Order Number (attach a copy of P.O. if applicable) \_\_\_\_\_

Authorized By:

Ship to:

**Joshua Smith** **Director**  
Name (Please Print) Title  
 **09-16-2020**  
Signature Date

CMI, Inc  
Attn: Service Dept.  
316 East Ninth Street  
Owensboro, KY 42303

Call: 405-425-2460 or email

No, please send estimate before repairs are made.

Note: An estimate will be faxed before performing any repairs and may cause delays in service.  
An evaluation fee (\$79.00 or actual costs) will apply to estimates that are not repaired.



DATE: 9/21/2020

316 E 9th Street / Owensboro KY 42303 / USA  
Phone: 866-835-0690 Fax: 270-685-6268

SERVICE WORK ORDER

405335

**Bill To:**  
Oklahoma Board Of Tests  
Blvd Adcu Annex Bldg #9  
3600 Martin Luther King  
Oklahoma City, OK 73136-3000  
USA  
Customer #: 731362  
Phone: 405-425-2424  
Fax: 405-425-2490 fax

**Ship To:**  
Oklahoma Board Of Tests  
Blvd Adcu Annex Bldg #9  
3600 Martin Luther King  
Oklahoma City OK 73136-3000  
USA  
Phone: 405-425-2424

MODEL #: 0024800K

Serial Number: 80-003395

BILL CODE: Out of Warranty

EXTRA PARTS RCVD:

BT,SHELF

DESCRIPTION OF PROBLEM

DIAGNOSTIC FAIL ON MODEM

WORK PERFORMED:

modem needed pins 24/36 cut; tested modem/ ok; replaced parts listed; calibrated/ final tested;

PARTS USED

Seq. No.	Part	Description	Quantity
50	410321	INSERT,M3.5 x 0.6,BRASS	1.00 EA
60	471201	O-RING,BUNA-N,-008,3/16inx5/16	1.00 EA
70	690040	BATTERY,3VOLT,LITHIUM,CR2032	1.00 EA
80	650517	CERTIFICATE OF CALIBRATION	2.00 EA
90	441169	COVER DUST,5/8in x 1/2in	1.00 EA
100	470145	CAP,PLASTIC,.25IDx.50LG,RED	3.00 EA
110	470154	CAP,PLSTC,.406IDx.438-.562,RED	1.00 EA
120	470218	SEAL,TAMPER EVIDENT,SERVICE	1.00 EA
140	923002	DIODE,SMD,1N4148,SOT-23	1.00 EA
150	402732	SCR,M3.5x12 PAN HD,PHIL,SST	1.00 EA
160	402752	SCR,M3.5X12 POZI CSK MC,BRIGHT	1.00 EA
170	402720	SCR,M4x12 FLAT HD,PHIL,SST	1.00 EA
180	530030	TUBING,TYGON,.375IDx.562OD	3.00 IN
190	470213	INSUL,PIPE,3/8inIDx3/8inTHKx72	1.00 IN
200	450151	TAG,S/N,CMI	1.00 EA
210	441098	SPCR,M3 X 4.5MM RD X 5MM LG	1.00 EA

LABOR / TESTING

Misc Code	Description	Hours
LABR	Service Repair Labor	
LCAL	Service - Calibration Adjust	0.50
LFT	Service - Cal / Final Test	1.00

Technician Name: Dewayne Varvel

SRV4053350001





# OFFICER'S AFFIDAVIT AND NOTICE OF REVOCATION/DISQUALIFICATION

11/16

Section 1

ARREST DATE 10/19/2020		ARREST TIME 1115		COUNTY # 55	CITY #	CITATION #		
ARREST LOCATION BOT					CITY	COUNTY OKLAHOMA		
SUBJECT NAME NORTH, GAYLON LEVERNE				DATE OF BIRTH 08/09/1961	SEX M	RACE W	HEIGHT 510	WEIGHT 165
ADDRESS 3600 MARTIN LUTHER KING A			CITY OKLAHOMA CITY		STATE OK	ZIP CODE 73133		
DRIVER LICENSE # T083454871			EXPIRATION DATE 06/30/2019	STATE OK	CLASS A	RESTRICTIONS	ENDORSEMENTS M	
VEHICLE MAKE MOCK		MODEL MOCK	TAG # MOCK		STATE OK	CMV N	PLACARD N	

On the above date, time, and location, the above named person was arrested, and I had reasonable grounds to believe the person was driving or in actual physical control of a motor vehicle upon a public road, highway, street, turnpike, public parking lot, or other public place, or upon a private road, street, alley or lane which provides access to one or more single or multi-family dwelling within this state while under the influence of alcohol and/or other intoxicating substances as prohibited by law.  
(Describe driving behavior or circumstances):


Describe person's condition (odor, actions, etc.):

MOCK SUBJECT TEST, POST REPAIR MAINTENANCE, INSTALL NEW CYLINDER

THE PERSON WAS INFORMED OF THE IMPLIED CONSENT TEST REQUEST

BREATH-ALCOHOL ANALYSIS RECORD, REPORT OF THE PERSON NAMED IN SECTION 1 ABOVE, and LOG OF TEST AND MAINTENANCE RECORD.

Section 2

EQUIPMENT I-8000		SERIAL NUMBER 80-003395	SPECIALIST BOARD OF TESTS																																					
STANDARD Dry		TARGET VALUE 0.080	PERMIT NUMBER 23020																																					
MANUFACTURER ILMO		LOT # 22620080A2	DATE CYLINDER INSTALLED 10/19/2020	DATE CYLINDER EXPIRES 10/05/2022																																				
OBSERVATION START 1130	TEST DATE 10/19/2020	MOUTHPIECE G	A 15-minute (or greater) deprivation/observation period was observed prior to and continuing to the time of test administration.  I administered said Breath-Alcohol Test in compliance with the applicable operating procedure of the Board of Tests.   SIGNATURE OF OPERATOR																																					
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.00</td><td>11:50</td></tr> <tr><td>Subject Test</td><td>0.00</td><td>11:50</td></tr> <tr><td>Breath Volume</td><td>1.515 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>11:50</td></tr> <tr><td>Wait</td><td></td><td>11:52</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>11:52</td></tr> <tr><td>Subject Test</td><td>0.00</td><td>11:53</td></tr> <tr><td>Breath Volume</td><td>1.601 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>11:53</td></tr> <tr><td>Cal Check</td><td>0.08</td><td>11:53</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>11:54</td></tr> </tbody> </table>					Test	g/210L	Time	Air Blank	0.00	11:50	Subject Test	0.00	11:50	Breath Volume	1.515 LITERS		Air Blank	0.00	11:50	Wait		11:52	Air Blank	0.00	11:52	Subject Test	0.00	11:53	Breath Volume	1.601 LITERS		Air Blank	0.00	11:53	Cal Check	0.08	11:53	Air Blank	0.00	11:54
Test	g/210L	Time																																						
Air Blank	0.00	11:50																																						
Subject Test	0.00	11:50																																						
Breath Volume	1.515 LITERS																																							
Air Blank	0.00	11:50																																						
Wait		11:52																																						
Air Blank	0.00	11:52																																						
Subject Test	0.00	11:53																																						
Breath Volume	1.601 LITERS																																							
Air Blank	0.00	11:53																																						
Cal Check	0.08	11:53																																						
Air Blank	0.00	11:54																																						
NAME PAPE, CHRISTOPHER			BADGE # 0000000484																																					
AGENCY BOARD OF TESTS			PERMIT # 0000023020																																					

**EFFECTIVE THIRTY (30) DAYS FROM DATE SERVED.** Notice of Revocation is given that your driver's license is revoked or denied for a period of one hundred eighty (180) days or more, if you refused or failed the state's test(s). In addition, your commercial driving privilege in this state will be disqualified if you refused or failed the state's test(s) (operating a CMV or CDL holder) OR a test result of .04 or more while operating a commercial motor vehicle. You may appeal any Departmental action against your driver license as a result of this arrest by filing a petition in the District Court of the County in which you were arrested. Your petition must be filed within thirty (30) days of the date listed below. You may be eligible to participate in the Impaired Driver Accountability Program (IDAP) administered by the Department of Public Safety (DPS). Completion of IDAP may prevent a revocation as a result of this arrest from appearing on your driving record. Participation in IDAP may reduce the amount of fees you will be required to pay to the State. You must request IDAP within thirty (30) days of the date listed below. Mail the request for IDAP to the Department of Public Safety at P.O. Box 11415, Oklahoma City, OK 73136.

Section 3

**SERVING OF NOTICE:** I personally hand delivered a copy of the above containing the Notice of Revocation and the Notice of Department Impaired Driving Accountability Program to the person named in Section 1 above.

Date served: **10/19/2020** Signature of officer: \_\_\_\_\_ Badge #: \_\_\_\_\_

In accordance with Title 12 O.S. Section 426, "I state under penalty of perjury under the laws of Oklahoma that the foregoing is true and correct."

Section 4

Date: **10/19/2020** Place (location when signed): \_\_\_\_\_ Signature of arresting officer: \_\_\_\_\_

NAME PAPE, CHRISTOPHER		AGENCY BOARD OF TESTS		
BADGE 0000000484	AGENCY ADDRESS INTER-AGENCY	ZIP CODE 00000	PHONE 4054252460	

OTHER WITNESSES:

Section 5

1	NAME	TITLE	ADDRESS	PHONE
2	NAME	TITLE	ADDRESS	PHONE

No Temporary License Issued:  
Test Below Legal Limit

OFFICER/DPS COPY  
BOT Form AFF01 03/2020



# OFFICER'S AFFIDAVIT AND NOTICE OF REVOCATION/DISQUALIFICATION

12/16

Section 1

ARREST DATE 10/19/2020		ARREST TIME 1115		COUNTY # 55	CITY #	CITATION #		
ARREST LOCATION BOT					CITY	COUNTY OKLAHOMA		
SUBJECT NAME NORTH, GAYLON LEVERNE				DATE OF BIRTH 08/09/1961	SEX M	RACE W	HEIGHT 510	WEIGHT 165
ADDRESS 3600 MARTIN LUTHER KING A			CITY OKLAHOMA CITY		STATE OK	ZIP CODE 73133		
DRIVER LICENSE # T083454871			EXPIRATION DATE 06/30/2019	STATE OK	CLASS A	RESTRICTIONS	ENDORSEMENTS M	
VEHICLE MAKE MOCK		MODEL MOCK	TAG # MOCK		STATE OK	CMV N	PLACARD N	

On the above date, time, and location, the above named person was arrested, and I had reasonable grounds to believe the person was driving or in actual physical control of a motor vehicle upon a public road, highway, street, turnpike, public parking lot, or other public place, or upon a private road, street, alley or lane which provides access to one or more single or multi-family dwelling within this state while under the influence of alcohol and/or other intoxicating substances as prohibited by law.  
(Describe driving behavior or circumstances):


Describe person's condition (odor, actions, etc.):

MOCK SUBJECT TEST, POST REPAIR MAINTENANCE, INSTALL NEW CYLINDER

**THE PERSON WAS INFORMED OF THE IMPLIED CONSENT TEST REQUEST**

BREATH-ALCOHOL ANALYSIS RECORD, REPORT OF THE PERSON NAMED IN SECTION 1 ABOVE, and LOG OF TEST AND MAINTENANCE RECORD.

Section 2

EQUIPMENT I-8000		SERIAL NUMBER 80-003395	SPECIALIST BOARD OF TESTS																																						
STANDARD Dry		TARGET VALUE 0.080	PERMIT NUMBER 23020																																						
MANUFACTURER ILMO		LOT # 22620080A2	DATE CYLINDER INSTALLED 10/19/2020	DATE CYLINDER EXPIRES 10/05/2022																																					
OBSERVATION START 1130	TEST DATE 10/19/2020	MOUTHPIECE G	A 15-minute (or greater) deprivation/observation period was observed prior to and continuing to the time of test administration.																																						
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.00</td><td>11:50</td></tr> <tr><td>Subject Test</td><td>0.00</td><td>11:50</td></tr> <tr><td>Breath Volume</td><td>1.515 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>11:50</td></tr> <tr><td>Wait</td><td></td><td>11:52</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>11:52</td></tr> <tr><td>Subject Test</td><td>0.00</td><td>11:53</td></tr> <tr><td>Breath Volume</td><td>1.601 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>11:53</td></tr> <tr><td>Cal Check</td><td>0.08</td><td>11:53</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>11:54</td></tr> </tbody> </table>			Test	g/210L	Time	Air Blank	0.00	11:50	Subject Test	0.00	11:50	Breath Volume	1.515 LITERS		Air Blank	0.00	11:50	Wait		11:52	Air Blank	0.00	11:52	Subject Test	0.00	11:53	Breath Volume	1.601 LITERS		Air Blank	0.00	11:53	Cal Check	0.08	11:53	Air Blank	0.00	11:54	<p>I administered said Breath-Alcohol Test in compliance with the applicable operating procedure of the Board of Tests.</p> <p style="text-align: center;"><i>Christopher Pape</i> 23020 SIGNATURE OF OPERATOR</p>		
Test	g/210L	Time																																							
Air Blank	0.00	11:50																																							
Subject Test	0.00	11:50																																							
Breath Volume	1.515 LITERS																																								
Air Blank	0.00	11:50																																							
Wait		11:52																																							
Air Blank	0.00	11:52																																							
Subject Test	0.00	11:53																																							
Breath Volume	1.601 LITERS																																								
Air Blank	0.00	11:53																																							
Cal Check	0.08	11:53																																							
Air Blank	0.00	11:54																																							
<table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td colspan="2">NAME PAPE, CHRISTOPHER</td> </tr> <tr> <td>BADGE # 0000000484</td> <td>PERMIT # 0000023020</td> </tr> <tr> <td colspan="2">AGENCY BOARD OF TESTS</td> </tr> </table>			NAME PAPE, CHRISTOPHER		BADGE # 0000000484	PERMIT # 0000023020	AGENCY BOARD OF TESTS																																		
NAME PAPE, CHRISTOPHER																																									
BADGE # 0000000484	PERMIT # 0000023020																																								
AGENCY BOARD OF TESTS																																									
<table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="text-align: center;">                 Test Result                  BrAC g/210L  <h2 style="margin: 0;">0.00</h2> </td> </tr> </table>			Test Result BrAC g/210L <h2 style="margin: 0;">0.00</h2>																																						
Test Result BrAC g/210L <h2 style="margin: 0;">0.00</h2>																																									

EFFECTIVE THIRTY (30) DAYS FROM DATE SERVED. Notice of Revocation is given that your driver's license is revoked or denied for a period of one hundred eighty (180) days or more, if you refused or failed the state's test(s). In addition, your commercial driving privilege in this state will be disqualified if you refused or failed the state's test(s) (operating a CMV or CDL holder) OR a test result of .04 or more while operating a commercial motor vehicle. You may appeal any Departmental action against your driver license as a result of this arrest by filing a petition in the District Court of the County in which you were arrested. Your petition must be filed within thirty (30) days of the date listed below. You may be eligible to participate in the Impaired Driver Accountability Program (IDAP) administered by the Department of Public Safety (DPS). Completion of IDAP may prevent a revocation as a result of this arrest from appearing on your driving record. Participation in IDAP may reduce the amount of fees you will be required to pay to the State. You must request IDAP within thirty (30) days of the date listed below. Mail the request for IDAP to the Department of Public Safety at P.O. Box 11415, Oklahoma City, OK 73136.

Section 3

**SERVING OF NOTICE:** I personally hand delivered a copy of the above containing the Notice of Revocation and the Notice of Department Impaired Driving Accountability Program to the person named in Section 1 above.

Date served: **10/19/2020** Signature of officer: \_\_\_\_\_ Badge #: \_\_\_\_\_

In accordance with Title 12 O.S. Section 426, "I state under penalty of perjury under the laws of Oklahoma that the foregoing is true and correct."

Section 4


Date: **10/19/2020** Place (location when signed): \_\_\_\_\_ Signature of arresting officer: \_\_\_\_\_

NAME PAPE, CHRISTOPHER		AGENCY BOARD OF TESTS	
BADGE 0000000484	AGENCY ADDRESS INTER-AGENCY	ZIP CODE 00000	PHONE 4054252460

No Temporary License Issued:  
Test Below Legal Limit

ARRESTEE'S COPY  
BQT Form AFF02 03/2020



Certificate of Analysis - Wet Bath	
8/11/2020	0.020
Date of Analysis	Labelled tank value (g/210L)
20070	0.020
Lot Number	Verifying result (g/210L)
	
BOT Technician Name and Signature	



**GUTH LABORATORIES, INC.**  
 150 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

BRT Form 6.0

In accordance with BRT - 2.2.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

**CERTIFICATE OF ANALYSIS**

ACV'D  
 6/11/2020  
 CP

ALPHA INSTRUMENT 2  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 80-004923  
 08/11/2020 09:42


**Certified Alcohol Reference Solution for Simulator**

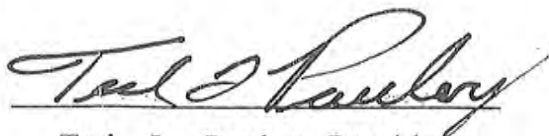
Test	g/210L	Time
Air Blank	0.000	09:42
Cal Check	0.020	09:43
Air Blank	0.000	09:43
Cal Check	0.020	09:44
Air Blank	0.000	09:45
Cal Check	0.020	09:45
Air Blank	0.000	09:46
Cal Check	0.020	09:47
Air Blank	0.000	09:47
Cal Check	0.021	09:48
Air Blank	0.000	09:48
Cal Check	0.020	09:49
Air Blank	0.000	09:49
Cal Check	0.020	09:50
Air Blank	0.000	09:51
Cal Check	0.020	09:51
Air Blank	0.000	09:52
Cal Check	0.020	09:53
Air Blank	0.000	09:53
Cal Check	0.019	09:54
Air Blank	0.000	09:54
Cal Check Stats		
Average	0.0200	
Std Dev	0.0004	
Rel Std Dev(%)	2.3569	

Random Samples of Lot Number **20070** of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on **February 17, 2020**, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain **0.0242%** (w/vol) ethyl alcohol. The expiration date for this lot number is **February 13, 2022** at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of **0.020 g/210L +/- 3%**.

The alcohol and water used in this solution were free of test interfering substances.

  
 Operator's Signature

  
 Ted L. Pauley, President  
 GUTH LABORATORIES, INC.

**NIST Traceability:**

Testing was conducted using Cerilliant Reference Standard lot number **FN08031603** whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.

Certificate of Analysis – Wet Bath	
7/22/2020	0.040
Date of Analysis	Labelled target value (g/210L)
20060	0.040
Lot Number	Average test result (g/210L)
Christopher Pauley	
BOT Technician Name and Signature	



14/16

**GUTH LABORATORIES, INC.**  
 100 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470  
 BRT Form 6.0

In accordance with BRT – 2.2.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

**CERTIFICATE OF ANALYSIS**

Certified Alcohol Reference Solution for Simulator

RCV'D  
6/1/20  
CP

Random Samples of Lot Number 20060 of

ALPHA UNIT SUB  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 80-003400  
 07/22/2020 14:57

Alcohol Reference Solution for Simulator were analyzed by gas chromatography on February 11, 2020, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.0483% (w/vol) ethyl alcohol. The expiration date for this lot number is February 10, 2022 at 11:59 PM.

Test	g/210L	Time
Air Blank	0.000	14:57
Cal Check	0.040	14:58
Air Blank	0.000	14:59
Cal Check	0.039	14:59
Air Blank	0.000	15:00
Cal Check	0.039	15:01
Air Blank	0.000	15:01
Cal Check	0.039	15:02
Air Blank	0.000	15:02
Cal Check	0.039	15:03
Air Blank	0.000	15:04
Cal Check	0.039	15:04
Air Blank	0.000	15:05
Cal Check	0.040	15:06
Air Blank	0.000	15:06
Cal Check	0.040	15:07
Air Blank	0.000	15:07
Cal Check	0.040	15:08
Air Blank	0.000	15:09
Cal Check	0.040	15:09
Air Blank	0.000	15:10
Cal Check Stats		
Average	0.0395	
Std Dev	0.0005	
Rel Std Dev(%)	1.3342	

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.040 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President  
 GUTH LABORATORIES, INC.

*Christopher Pauley*  
 Operator's Signature

**NIST Traceability:**

Testing was conducted using Cerilliant Reference Standard lot number FN12181501 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.



Certificate of Analysis - wet Data



15/16

06/16/20	.100
Date of Analysis	Labelled target value (g/210L)
20190	.098
Lot Number	Average test result (g/210L)
Josh Smith	
BOT Technician Name and Signature	

GUTH LABORATORIES, INC.

1001 BRT Form 6.0 GUTH LABORATORIES, INC. RISE JRG, PA 17111-4511 • TELEPHONE: 717-564-5470

In accordance with BRT - 2.2.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

Rec'd  
06/11/2020  
*[Signature]*

CERTIFICATE OF ANALYSIS

ALPHA INSTRUMENT  
Intoxilyzer - Alcohol Analyzer  
Model 8000  
06/16/2020

SN 80-002591  
16:18

Certified Alcohol Reference Solution for Simulator

Test	g/210L	Time
Air Blank	0.000	16:18
Cal Check	0.099	16:19
Air Blank	0.000	16:20
Cal Check	0.098	16:20
Air Blank	0.000	16:21
Cal Check	0.097	16:22
Air Blank	0.000	16:22
Cal Check	0.098	16:23
Air Blank	0.000	16:24
Cal Check	0.098	16:24
Air Blank	0.000	16:25
Cal Check	0.098	16:26
Air Blank	0.000	16:26
Cal Check	0.098	16:27
Air Blank	0.000	16:27
Cal Check	0.097	16:28
Air Blank	0.000	16:29
Cal Check	0.098	16:29
Air Blank	0.000	16:30
Cal Check	0.098	16:31
Air Blank	0.000	16:31
Cal Check Stats		
Average	0.0979	
Std Dev	0.0005	
Rel Std Dev(%)	0.5798	

Random Samples of Lot Number 20190 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on April 8, 2020, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1206% (w/vol) ethyl alcohol. The expiration date for this lot number is April 6, 2022 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

*[Signature]* 16037  
Operator's Signature

*[Signature]*  
Ted L. Pauley, President  
GUTH LABORATORIES, INC.

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN02271802 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.

Certificate of Analysis - Wet Bath	
07/07/2020	0.200
Date of Analysis	Labeled Weight Value (g/210L)
20160	0.197
Lot Number	Average Test Result (g/210L)
Christopher Pope	23030
BOT Technician Name and Signature	



**GUTH LABORATORIES, INC.**  
 550 NORTH 6TH STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-584-5470

BRT Form 6.0

In accordance with BRT - 2.2.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

### CERTIFICATE OF ANALYSIS

*REC'D  
05/2020  
CP*

#### Certified Alcohol Reference Solution for Simulator

LPHR UNIT SUB  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 80-003400  
 7/07/2020 15:25

Test	g/210L	Time
ir Blank	0.000	15:26
al Check	0.196	15:26
ir Blank	0.000	15:27
al Check	0.196	15:28
ir Blank	0.000	15:28
al Check	0.197	15:29
ir Blank	0.000	15:29
al Check	0.196	15:30
ir Blank	0.000	15:31
al Check	0.198	15:31
ir Blank	0.000	15:32
al Check	0.198	15:33
ir Blank	0.000	15:33
al Check	0.197	15:34
ir Blank	0.000	15:35
al Check	0.198	15:35
ir Blank	0.000	15:36
al Check	0.198	15:37
ir Blank	0.000	15:37
al Check	0.197	15:38
ir Blank	0.000	15:38
al Check Stats		
Average	0.1971	
Std Dev	0.0008	
Rel Std Dev(%)	0.4442	

Random Samples of Lot Number **20160** of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on March 20, 2020, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain **0.2427%** (w/vol) ethyl alcohol. The expiration date for this lot number is **March 18, 2022** at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of **0.200 g/210L +/- 3%**.

The alcohol and water used in this solution were free of test interfering substances.

*Christopher Pope*  
 Operator's Signature

*Ted L. Pauley*  
 Ted L. Pauley, President  
 GUTH LABORATORIES, INC.

#### NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN08101505 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.