



**STATE OF OKLAHOMA  
BOARD OF TESTS FOR ALCOHOL AND DRUG INFLUENCE**

Post Office Box 36307

Oklahoma City, Oklahoma 73136-2307  
Phone: (405) 425-2460 Fax: (405) 425-2490  
www.bot.ok.gov

Dr. Jarrad Wagner, Ph.D. F-ABFT  
Chairman


Joshua Smith  
Director

ATTESTATION

I, the undersigned Joshua Smith (Director/Records Custodian), attest under oath pursuant to 12 O.S. §2902 (11)(a) this record was made, at or near the time of the occurrence of the matters set forth by or from information transmitted by a person having knowledge of those matters; was kept in the course of the regularly conducted business activity of the Board; and was made pursuant to the regularly conducted activity. The duplicate record provided is listed below:

- 1) The attached "Service Overview" is a true and accurate copy of maintenance performed on the Intoxilyzer 8000, serial number 80-003400, in compliance with the agency's Maintenance Policy and Procedures.

This packet consists of 14 pages.

Signed 

Name of Position: Director/Records Custodian

Date of Attestation: 05/19/2022

# Service Overview

Board of Tests for Alcohol and Drug Influence  
Ensuring public safety by ensuring the accuracy and reliability  
of breath and blood testing



3600 N. Martin Luther King Bldg #9  
Oklahoma City, OK 73111  
405-425-2460

**BENCH CHECK DATE:** 06-06-2019

**SERIAL:** 80-003400

## **DOCUMENTATION WITHIN SERVICE PACKET:**

- BOT Certificate of Calibration and Operation
- Bench Check
- Bench Check Technician's Report
- BOT Dry Gas Certificate of Analysis
- Mock Subject Test
- BOT Certificates of Analysis on Certified Solutions (4)



Date:

Re: Request for Log of Test on Intoxilyzer 8000

Name:

Dear Sir:

The Log of Test information from a breath test conducted on a Intoxilyzer 8000 is printed in Section 2 of the Affidavit and is no longer retained as a separate form as with the Intoxilyzer 5000. The 8000 uses a nitrogen/ethanol dry gas for the external control test. The dry gas cylinder has the capacity to perform approximately 325 tests and does not require maintenance until its expiration date or can no longer provide the required pressure to perform a control test. The cylinder has an expiration date of two years from date filled at the manufacturer and is programmed in the 8000 upon installation, both dates are printed in Section 2 of the Affidavit. The Intoxilyzer is programmed to disable itself when the date of expiration is reached or the pressure monitor indicates 25 lbs psi.

Due to the reliability and stability of dry gas, maintenance on the 8000 is not required every 30 days or 25 tests, therefore maintenance is no longer performed by officers in the field. The Board of Tests for Alcohol and Drug Influence certifies each Intoxilyzer 8000 for field use by performing a bench check. The bench check is designed to check the operation and procedures programmed in the 8000 to ensure it is functioning properly for use in Oklahoma. A bench check is performed every time a new dry gas cylinder is installed or the instrument has returned from the manufacturer for repair. Once the instrument passes the bench check, all that is required to set it up for field use is to plug it in and turn it on and does not require a permit to set up. The Board of Tests has the ability to monitor each instrument once it is set up in the field.

Each Intoxilyzer has a database of valid permit numbers that it checks prior to allowing a breath test to be performed. The database is updated on a regular basis, if a permit number is invalid that officer will not be able to conduct a breath test on the 8000. If the 8000 prints an affidavit the breath test operator listed in Section 2 had a valid permit at the time of the test and the breath test is valid.

If you have any further questions please feel free to call me.

Sincerely,



J. Robert Blakeburn (OBA11059)  
State Director of Tests for Alcohol  
and Drug Influence

**STATE OF OKLAHOMA - BOARD OF TESTS FOR ALCOHOL AND DRUG INFLUENCE  
CMI INTOXILYZER BENCH CHECK PROCEDURE REPORT**

BENCH CHECK DATE 06/06/2019	TIME PROCEDURE BEGAN 09:21:1	INSTRUMENT LOCATION 80-003400
INSTRUMENT TYPE Intoxilyzer	INSTRUMENT MODEL I-8000	INSTRUMENT SERIAL NUMBER 80-003400

**TEST RESULTS**

**Diagnostics**

PASS

**Mouth Alcohol Test**

PASS

**RFI Test**

PASS

**Abort Test**

PASS

**Improper Sample Test**

PASS

**Interferent Detect Test**

PASS

**No Sample Given Test**

PASS

**Insufficient Sample Test**

PASS

**Air Blank Contamination Test**

PASS

**Range Exceeded Test**

PASS


**Duplicate Breath Sampling Results**

Value	Test 1	Test 2	Control Test
.02	0.015	0.015	0.016
.04	0.037	0.037	0.038
.10	0.101	0.100	0.101
.20	0.203	0.202	0.202

PASS

**CERTIFYING TECHNICIAN**

I swear under penalty of perjury that in regards to the above listed instrument, I have complied with the Intoxilyzer Bench Checking Procedure approved by the State of Oklahoma.

SIGNATURE 	DATE 06/06/19
NAME SMITH, JOSHUA	PERMIT # 0000016837



Board of Tests for Alcohol and Drug Influence  
Enhancing public safety by ensuring the accuracy and scientific reliability  
of blood and breath testing



3600 N. Martin Luther King Bldg #9  
Oklahoma City, OK 73111  
405-425-2460

# BENCH CHECK TECHNICIAN'S REPORT

Date: 06/06/19 Start Time: 0920 End Time: 1047

## INSTRUMENT

Intoxilyzer Model 8000 Serial # 80-003400

## GAS CANISTER

LOT # 06419080A2 # 039 EXP Date 05/05/2021

## REFERENCE

Simulator Model			
Guth 2100	Guth 2100	Guth 2100	Guth 2100
Serial #			
DR3591	DR3753	DR3594	DR3754
Concentration			
.02	.04	.10	.20
LOT #			
18020	17410	18070	17340
Manufactured Date			
01-09-2018	12-06-2017	02-26-2018	10-09-2017
Expiration Date			
01-09-2020	12-06-2019	02-26-2020	10-09-2019
Solution Commission Date			
<u>06-06-19</u>	<u>06-06-19</u>	<u>06-06-19</u>	<u>06-06-19</u>

## REASON FOR BENCH CHECK


- POST REPAIR
- CYLINDER REPLACEMENT
- TROUBLESHOOTING
- ROUTINE MAINTENANCE

## COMMENTS


[Signature] 16837  
Technician Signature / Permit #

Josh Smith  
Printed Name

Certificate of Analysis - Dry Gas	
05-31-19	.080
Date of Analysis	Labelled target value (g/210L)
039	.080
Cylinder #	Average test result
Josth Smith	
BOT Technician Name and Signature	

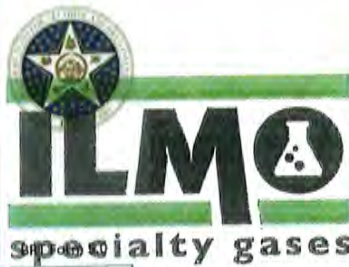

7/14  
 ALPHA INSTRUMENT  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 80-002591  
 05/31/2019 14:28

In accordance with BOT Policy and Procedure Statement BRT-2.1.0, Maintenance, the above referenced dry gas cylinder is suitable for use as an external reference gas cylinder for the following:

75 East Ninth St. P.O. Box 790 • Jacksonville, IL 62651-0790  
 217-245-2183 • Fax: 217-243-7634 • www.ilmoproducts.com

Test	g/210L	Time
Air Blank	0.000	14:29
Cal Check	0.079	14:29
Air Blank	0.000	14:29
Cal Check	0.079	14:29
Air Blank	0.000	14:30
Cal Check	0.080	14:31
Air Blank	0.000	14:31
Cal Check	0.080	14:31
Air Blank	0.000	14:32
Cal Check	0.079	14:32
Air Blank	0.000	14:33
Cal Check	0.080	14:33
Air Blank	0.000	14:34
Cal Check	0.080	14:34
Air Blank	0.000	14:35
Cal Check	0.079	14:35
Air Blank	0.000	14:35
Cal Check	0.080	14:36
Air Blank	0.000	14:36
Cal Check	0.079	14:37
Air Blank	0.000	14:37
Cal Check Stats		
Average	0.0795	
Std Dev	0.0005	
Rel Std Dev(%)	0.6629	

## Certificate of Analysis

Certificate ID: 11860  
 Part #: BAC105L080T  
 Cylinder Size: 105L  
 Lot Number: 06419080A2 ✓  
 Expiration: 5/5/2021 ✓

REC'D  
 05/22/19

0.080 BAC (For the calibration of instruments used to determine breath alcohol concentration)

Contents: 105 Liters @ 1000 psig 70°F (21°C)

Component:	Reported Concentration:	Analytical Accuracy (U, k=2):	Analytical Method:
Ethanol	208 ppm	+/-0.002 BAC(G/210L) [5.2 ppm]	NDIR
Nitrogen	Balance		

Distributed by:

CMI Inc.  
 316 East Ninth Str  
 Owensboro, KY 4  
 Phone 866-835-06  
[www.alcoholtest.com](http://www.alcoholtest.com)

Operator's Signature 16837

\*NIST Traceable Reference Material  
 Cylinder No. CC274523 / Job No. 09160306  
 Certified 362.2 µmol/mol Ethanol in Nitrogen

Store in dry area, away from sources of heat, ignition and direct sunlight. Do not allow storage area to exceed 52 °C (125 °F).

Specialist Gas Lab Tech

03-19-19  
 Date



The calibration results within this certificate were obtained using equipment and standards capable of producing analytical results traceable to NIST, and apply only to the items contained on this certificate. ILMO Products Company makes no warranty or representation as to the suitability of the use of any information provided for any particular purpose. The information use is at the sole discretion and risk of the user. Liability shall be limited to established replacement cost of this material or service.

ISO/IEC 17025:2005 Accredited Laboratory



# OFFICER'S AFFIDAVIT AND NOTICE OF REVOCATION/DISQUALIFICATION

Section 1

ARREST DATE <b>06/06/2019</b>		ARREST TIME <b>1000</b>		COUNTY # <b>55</b>	CITY # <b>52</b>	CITATION # <b>NON</b>		
ARREST LOCATION <b>NONE</b>				CITY <b>NONE</b>		COUNTY <b>OKLAHOMA</b>		
SUBJECT NAME <b>MOCK , SUBJECT TEST</b>				DATE OF BIRTH <b>08/09/1961</b>	SEX <b>M</b>	RACE <b>W</b>	HEIGHT <b>510</b>	WEIGHT <b>165</b>
ADDRESS <b>3600 MARTIN LUTHER KING A</b>			CITY <b>OKLAHOMA CITY</b>		STATE <b>OK</b>	ZIP CODE <b>73133</b>		
DRIVER LICENSE # <b>T083454871</b>			EXPIRATION DATE <b>06/30/2019</b>	STATE <b>OK</b>	CLASS <b>A</b>	RESTRICTIONS	ENDORSEMENTS <b>M</b>	
VEHICLE MAKE <b>NONE</b>		MODEL <b>NONE</b>	TAG # <b>NONE</b>		STATE <b>OK</b>	CMV <b>N</b>	PLACARD <b>N</b>	

On the above date, time, and location, the above named person was arrested, and I had reasonable grounds to believe the person was driving or in actual physical control of a motor vehicle upon a public road, highway, street, turnpike, public parking lot, or other public place, or upon a private road, street, alley or lane which provides access to one or more single or multi-family dwelling within this state while under the influence of alcohol and/or other intoxicating substances as prohibited by law.

(Describe driving behavior or circumstances):


**MOCK SUBJECT TEST. ROUTINE MAINTENANCE, NEW GAS CANISTER INSTALL**

Describe person's condition (odor, actions, etc.):

THE PERSON WAS INFORMED OF THE IMPLIED CONSENT TEST REQUEST

Section 2

BREATH-ALCOHOL ANALYSIS RECORD, REPORT OF THE PERSON NAMED IN SECTION 1 ABOVE, and LOG OF TEST AND MAINTENANCE RECORD.

EQUIPMENT <b>I-8000</b>		SERIAL NUMBER <b>80-003400</b>	SPECIALIST <b>BOARD OF TESTS</b>																																								
STANDARD <b>Dry</b>		TARGET VALUE <b>0.080</b>	PERMIT NUMBER <b>16837</b>																																								
MANUFACTURER <b>ILMO</b>		LOT # <b>06419080A2</b>	DATE CYLINDER INSTALLED <b>06/06/2019</b>	DATE CYLINDER EXPIRES <b>05/05/2021</b>																																							
OBSERVATION START <b>1010</b>	TEST DATE <b>06/06/2019</b>	MOUTHPIECE <b>G</b>	A 15-minute (or greater) deprivation/observation period was observed prior to and continuing to the time of test administration.																																								
RESULT TABLE <table style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="text-align: left;">Test</th> <th style="text-align: left;">g/210L</th> <th style="text-align: left;">Time</th> </tr> </thead> <tbody> <tr><td colspan="3">-----</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:48</td></tr> <tr><td>Subject Test</td><td>0.29</td><td>10:49</td></tr> <tr><td>  Breath Volume</td><td>1.691 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:49</td></tr> <tr><td>Wait</td><td></td><td>10:51</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:51</td></tr> <tr><td>Subject Test</td><td>0.29</td><td>10:52</td></tr> <tr><td>  Breath Volume</td><td>3.015 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:53</td></tr> <tr><td>Cal Check</td><td>0.07</td><td>10:53</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:54</td></tr> </tbody> </table>					Test	g/210L	Time	-----			Air Blank	0.00	10:48	Subject Test	0.29	10:49	Breath Volume	1.691 LITERS		Air Blank	0.00	10:49	Wait		10:51	Air Blank	0.00	10:51	Subject Test	0.29	10:52	Breath Volume	3.015 LITERS		Air Blank	0.00	10:53	Cal Check	0.07	10:53	Air Blank	0.00	10:54
Test	g/210L	Time																																									
-----																																											
Air Blank	0.00	10:48																																									
Subject Test	0.29	10:49																																									
Breath Volume	1.691 LITERS																																										
Air Blank	0.00	10:49																																									
Wait		10:51																																									
Air Blank	0.00	10:51																																									
Subject Test	0.29	10:52																																									
Breath Volume	3.015 LITERS																																										
Air Blank	0.00	10:53																																									
Cal Check	0.07	10:53																																									
Air Blank	0.00	10:54																																									
SIGNATURE OF OPERATOR																																											
NAME <b>SMITH, JOSHUA</b>			  Test Result BrAC g/210L <b>0.29</b>																																								
BADGE # <b>0000000435</b>		PERMIT # <b>0000016837</b>																																									
AGENCY <b>BOARD OF TESTS</b>																																											

**EFFECTIVE THIRTY (30) DAYS FROM DATE SERVED.** Notice of Revocation is given that your driver's license is revoked or denied for a period of one hundred eighty (180) days or more, if you refused or failed the state's test(s). In addition, your commercial driving privilege in this state will be disqualified if you refused or failed the state's test(s) (operating a CMV or CDL holder) OR a test result of .04 or more while operating a commercial motor vehicle. To appeal the driver's license revocation/disqualification, the Department of Public Safety must receive your written request for an administrative hearing on the Department approved form, within fifteen (15) days from the date you received notice of revocation or disqualification. The approved hearing request form is available at <https://www.ok.gov/dps/documents/ReqHearing.pdf>. Submit your hearing request form in person at 3600 N. MLK Ave. or by mail to Legal Division, Department of Public Safety, P.O. Box 11415, OKC, OK 73136. It shall be a misdemeanor punishable by imprisonment for not less than seven (7) days nor more than six (6) months, or by a fine of not more than Five Hundred Dollars (\$500.00), or by both such fine and imprisonment, for any person to apply for a renewal or a replacement license to operate a motor vehicle while the person's license, permit, or other evidence of driving privilege is in the custody of a law enforcement officer or the Department.

**SERVING OF NOTICE:** I personally hand-delivered a copy of the above containing the Notice of Revocation to the person named in Section 1 above.

Date served: **06/06/2019** Signature of officer: \_\_\_\_\_ Badge #: \_\_\_\_\_

In accordance with Title 12 O.S. Section 426, "I state under penalty of perjury under the laws of Oklahoma that the foregoing is true and correct."

Date: **06/06/2019** Place (location when signed): \_\_\_\_\_ Signature of arresting officer: \_\_\_\_\_

NAME <b>SMITH, JOSHUA</b>		AGENCY <b>BOARD OF TESTS</b>	
BADGE <b>0000000435</b>	AGENCY ADDRESS <b>INTER-AGENCY</b>	ZIP CODE <b>00000</b>	PHONE <b>"4054252460"</b>

OTHER WITNESSES:

	NAME	TITLE	ADDRESS	PHONE
1				
2				

Temporary License Issued

OFFICER/DPS COPY  
BOT Form AFF01 01/2019



# OFFICER'S AFFIDAVIT AND NOTICE OF REVOCATION/DISQUALIFICATION

Section 1

ARREST DATE 06/06/2019		ARREST TIME 1000		COUNTY # 55		CITY # 52		CITATION # NON	
ARREST LOCATION NONE				CITY NONE			COUNTY OKLAHOMA		
SUBJECT NAME MOCK , SUBJECT TEST				DATE OF BIRTH 08/09/1961		SEX M	RACE W	HEIGHT 510	WEIGHT 165
ADDRESS 3600 MARTIN LUTHER KING A				CITY OKLAHOMA CITY			STATE OK		ZIP CODE 73133
DRIVER LICENSE # T083454871		EXPIRATION DATE 06/30/2019		STATE OK	CLASS A	RESTRICTIONS		ENDORSEMENTS M	
VEHICLE MAKE NONE		MODEL NONE		TAG # NONE		STATE OK	CMV N	PLACARD N	

On the above date, time, and location, the above named person was arrested, and I had reasonable grounds to believe the person was driving or in actual physical control of a motor vehicle upon a public road, highway, street, turnpike, public parking lot, or other public place, or upon a private road, street, alley or lane which provides access to one or more single or multi-family dwelling within this state while under the influence of alcohol and/or other intoxicating substances as prohibited by law.

(Describe driving behavior or circumstances):

MOCK SUBJECT TEST. ROUTINE MAINTENANCE, NEW GAS CANISTER INSTALL

Describe person's condition (odor, actions, etc.):

### THE PERSON WAS INFORMED OF THE IMPLIED CONSENT TEST REQUEST

BREATH-ALCOHOL ANALYSIS RECORD, REPORT OF THE PERSON NAMED IN SECTION 1 ABOVE, and LOG OF TEST AND MAINTENANCE RECORD.

Section 2

EQUIPMENT I-8000		SERIAL NUMBER 80-003400		SPECIALIST BOARD OF TESTS																																								
STANDARD Dry		TARGET VALUE 0.080		PERMIT NUMBER 16837																																								
MANUFACTURER ILMO		LOT # 06419080A2		DATE CYLINDER INSTALLED 06/06/2019	DATE CYLINDER EXPIRES 05/05/2021																																							
OBSERVATION START 1010	TEST DATE 06/06/2019	MOUTHPIECE G	A 15-minute (or greater) deprivation/observation period was observed prior to and continuing to the time of test administration.																																									
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>-----</td><td>-----</td><td>-----</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:48</td></tr> <tr><td>Subject Test</td><td>0.29</td><td>10:49</td></tr> <tr><td>  Breath Volume</td><td>1.691 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:49</td></tr> <tr><td>Wait</td><td></td><td>10:51</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:51</td></tr> <tr><td>Subject Test</td><td>0.29</td><td>10:52</td></tr> <tr><td>  Breath Volume</td><td>3.015 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:53</td></tr> <tr><td>Cal Check</td><td>0.07</td><td>10:53</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:54</td></tr> </tbody> </table>						Test	g/210L	Time	-----	-----	-----	Air Blank	0.00	10:48	Subject Test	0.29	10:49	Breath Volume	1.691 LITERS		Air Blank	0.00	10:49	Wait		10:51	Air Blank	0.00	10:51	Subject Test	0.29	10:52	Breath Volume	3.015 LITERS		Air Blank	0.00	10:53	Cal Check	0.07	10:53	Air Blank	0.00	10:54
Test	g/210L	Time																																										
-----	-----	-----																																										
Air Blank	0.00	10:48																																										
Subject Test	0.29	10:49																																										
Breath Volume	1.691 LITERS																																											
Air Blank	0.00	10:49																																										
Wait		10:51																																										
Air Blank	0.00	10:51																																										
Subject Test	0.29	10:52																																										
Breath Volume	3.015 LITERS																																											
Air Blank	0.00	10:53																																										
Cal Check	0.07	10:53																																										
Air Blank	0.00	10:54																																										
RESULT TABLE			SIGNATURE OF OPERATOR _____																																									
			NAME SMITH, JOSHUA																																									
			BADGE # 0000000435	PERMIT # 0000016837																																								
			AGENCY BOARD OF TESTS																																									



Test Result  
BrAC g/210L  
**0.29**

**EFFECTIVE THIRTY (30) DAYS FROM DATE SERVED.** Notice of Revocation is given that your driver's license is revoked or denied for a period of one hundred eighty (180) days or more, if you refused or failed the state's test(s). In addition, your commercial driving privilege in this state will be disqualified if you refused or failed the state's test(s) (operating a CMV or CDL holder) OR a test result of .04 or more while operating a commercial motor vehicle. To appeal the driver's license revocation/disqualification, the Department of Public Safety must receive your written request for an administrative hearing on the Department approved form, within fifteen (15) days from the date you received notice of revocation or disqualification. **The approved hearing request form is available at <https://www.ok.gov/dps/documents/ReqHearing.pdf>.** Submit your hearing request form in person at 3600 N. MLK Ave. or by mail to Legal Division, Department of Public Safety, P.O. Box 11415, OKC, OK 73136. It shall be a misdemeanor punishable by imprisonment for not less than seven (7) days nor more than six (6) months, or by a fine of not more than Five Hundred Dollars (\$500.00), or by both such fine and imprisonment, for any person to apply for a renewal or a replacement license to operate a motor vehicle while the person's license, permit, or other evidence of driving privilege is in the custody of a law enforcement officer or the Department.

Section 3

**SERVING OF NOTICE:** I personally hand-delivered a copy of the above containing the Notice of Revocation to the person named in Section 1 above.

Date served: **06/06/2019** Signature of officer: \_\_\_\_\_ Badge #: \_\_\_\_\_

In accordance with Title 12 O.S. Section 426, "I state under **penalty of perjury** under the laws of Oklahoma that the foregoing is true and correct."

Section 4

Date: **06/06/2019** Place (location when signed): \_\_\_\_\_ Signature of arresting officer: \_\_\_\_\_

NAME SMITH, JOSHUA		AGENCY BOARD OF TESTS	
BADGE 0000000435	AGENCY ADDRESS INTER-AGENCY	ZIP CODE 00000	PHONE "4054252460"

Temporary License Issued

ARRESTEE'S COPY  
BOT Form AFF02 01/2019

# STATE OF OKLAHOMA - DEPARTMENT OF PUBLIC SAFETY

## Receipt for Driver License and Temporary Driving Permit

**.02 or Greater BrAC for under 21 yoa, 0.08 or Greater BrAC for 21 yoa and older, or REFUSAL**

DATE OF ARREST 06/06/2019		TIME OF ARREST 1000	
NAME (LAST, FIRST, MIDDLE) MOCK , SUBJECT TEST			
ADDRESS 3600 MARTIN LUTHER KING A			
CITY OKLAHOMA CITY		STATE OK	ZIP CODE 73133
DRIVER LICENSE NUMBER T083454871	STATE OK	BIRTHDATE 08/09/1961	SEX M
		RACE W	WEIGHT 165
			HEIGHT 510
CLASS A	EXPIRATION 06/30/2019	RESTRICTIONS	ENDORSEMENTS M

BrAC  
**0.29**

DATE ISSUED: 06/06/2019

**This form is valid as a driver permit for a period of thirty (30) days from the date it was issued.**

Anyone using this form thirty (30) days after issuance may be driving under suspension. All law enforcement officers may determine if the holder is driving under suspension by requesting a Driver's License status through OLETS. This receipt and permit is issued to individuals who have refused to take or have taken a breath test to determine Alcohol Content and the results indicated a Breath Alcohol Content as specified under the Implied Consent Law and Title 47, 11-902, and/or 11-906.4.

### VIOLATOR'S REVOCATION NOTICE

Upon receipt of a written blood or breath test report reflecting that the arrested person, if under twenty-one (21) years of age, had any measurable quantity of alcohol in the person's blood or breath, or, if the arrested person is twenty-one (21) years of age or older, a blood or breath alcohol concentration of eight-hundredths (0.08) or more, or refused the State's test, accompanied by a sworn report from a law enforcement officer that the officer had reasonable grounds to believe the arrested person had been operating or was in actual physical control of a motor vehicle while under the influence of alcohol as prohibited by law, the Department shall revoke or deny the driving privilege of the arrested person for a period as provided by Section 6-205.1 of Title 47. Revocation or denial of the driving privilege of the arrested person shall become effective thirty (30) days after the arrested person is given written notice thereof by the officer as provided in this section or by the Department as provided in Section 2-116 of Title 47.

Upon the written request of the person whose driving privilege has been revoked or denied by this notice, the Department of Public Safety shall grant the person an opportunity to be heard if the request is received by the Department within fifteen (15) days after the notice. The sworn report of the officer, together with the results of any test or tests, shall be deemed true, absent any facial deficiency, should the requesting person fail to appear at the scheduled hearing.

It shall be a misdemeanor punishable by imprisonment for not less than seven (7) days nor more than six (6) months, or by a fine of not more than Five Hundred Dollars (\$500.00), or by both such fine and imprisonment, for any person to apply for a renewal or a replacement license to operate a motor vehicle while the person's license, permit, or other evidence of driving privilege is in the custody of a law enforcement officer or the Department.

ARRESTING OFFICER	
SIGNATURE	BADGE NUMBER 000000435
SMITH, JOSHUA	AGENCY BOARD OF TESTS



**GUTH LABORATORIES, INC.**  
 590 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-6470

Certificate of Analysis – Wet Bath	
09-26-2018	0.0200
Date of Analysis	Labelled target value (g/210L)
18020	0.0204
Lot Number	Average test result (g/210L)
BOT Technician Name and Signature Josh Smith	



BRT Form 6.0

In accordance with BRT – 2.1.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

**CERTIFICATE OF ANALYSIS**

Certified Alcohol Reference Solution for Simulator

RECV'D  
08/25/18  
[Signature]

Random Samples of Lot Number 18020 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on January 11, 2018, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.0238% (w/vol) ethyl alcohol. The expiration date for this lot number is January 9, 2020 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.020 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

ALPHA INSTRUMENT  
Intoxilyzer – Alcohol Analyzer  
Model 8000  
09/26/2018

SN 80-002591  
15:36

Test	g/210L	Time
Air Blank	0.000	15:36
Cal Check	0.020	15:37
Air Blank	0.000	15:37
Cal Check	0.020	15:38
Air Blank	0.000	15:39
Cal Check	0.020	15:39
Air Blank	0.000	15:40
Cal Check	0.020	15:41
Air Blank	0.000	15:41
Cal Check	0.020	15:42
Air Blank	0.000	15:42
Cal Check	0.020	15:43
Air Blank	0.000	15:44
Cal Check	0.021	15:44
Air Blank	0.000	15:45
Cal Check	0.021	15:46
Air Blank	0.000	15:46
Cal Check	0.021	15:47
Air Blank	0.000	15:47
Cal Check	0.021	15:48
Air Blank	0.000	15:49
Cal Check Stats		
Average	0.0204	
Std Dev	0.0005	
Rel Std Dev(%)	2.5312	

[Signature] 16837  
Operator's Signature

[Signature]  
Ted L. Pauley, President  
GUTH LABORATORIES, INC.

**NIST Traceability:**  
 Testing was conducted using Cerilliant Reference Standard lot number FN08031603 whose values are traceable to NIST.  
 All balances are calibrated annually by an outside agency using NIST traceable weights.  
 Calibration verification is done prior to each use utilizing NIST traceable weights.





**GUTH LABORATORIES, INC.**  
 590 NORTH 67th STREET • HARRISBURG, PA 17111-2511 • TELEPHONE: 717-664-5470

12/14

Certificate of Analysis - Wet Bath	
Date of Analysis	09-26-18
Labelled target value (g/210L)	.040
Lot Number	17410
Average test result (g/210L)	0.0396
BOT Technician Name and Signature	
Josh Smith	

In accordance with BRT - 2.1.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.



BRT Form 6.0

**CERTIFICATE OF ANALYSIS**

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 17410 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on December 7, 2017, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.0481% (w/vol) ethyl alcohol. The expiration date for this lot number is December 6, 2019 at 11:59 PM.

RECD  
8/25/18  
JR

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.040 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

ALPHA INSTRUMENT  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 00-002591  
 09/26/2018 15:54

Test	g/210L	Time
Air Blank	0.000	15:54
Cal Check	0.040	15:55
Air Blank	0.000	15:56
Cal Check	0.039	15:56
Air Blank	0.000	15:57
Cal Check	0.039	15:58
Air Blank	0.000	15:58
Cal Check	0.040	15:59
Air Blank	0.000	15:59
Cal Check	0.040	16:00
Air Blank	0.000	16:01
Cal Check	0.040	16:01
Air Blank	0.000	16:02
Cal Check	0.039	16:03
Air Blank	0.000	16:03
Cal Check	0.040	16:04
Air Blank	0.000	16:04
Cal Check	0.040	16:05
Air Blank	0.000	16:06
Cal Check	0.039	16:06
Air Blank	0.000	16:07
Cal Check Stats		
Average	0.0396	
Std Dev	0.0005	
Rel Std Dev(%)	1.3040	

16837  
 Operator's Signature


Ted L. Pauley, President  
 GUTH LABORATORIES, INC.

**NIST Traceability:**

Testing was conducted using Cerilliant Reference Standard lot number FN12181501 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.



Certificate of Analysis - Wet Bath	
09-27-2018	.100
Date of Analysis	Labelled Target value (g/210L)
18070	0.0996
Lot Number	Actual Test Result (g/210L)
	
BOT Technician Name and Signature	



**GUTH LABORATORIES, INC.**  
 590 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

BRT Form 6.0


In accordance with BRT - 2.1.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

**CERTIFICATE OF ANALYSIS**

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 18070 of

Alcohol Reference Solution for Simulator were analyzed by gas chromatography on February 28, 2018, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1219% (w/vol) ethyl alcohol. The expiration date for this lot number is February 26, 2020 at 11:59 PM.

REC'D  
02/25/18  



When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.


ALPHA INSTRUMENT  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 00-002591  
 09/27/2018 08:28

Test	g/210L	Time
Air Blank	0.000	08:28
Cal Check	0.100	08:29
Air Blank	0.000	08:29
Cal Check	0.100	08:30
Air Blank	0.000	08:31
Cal Check	0.099	08:31
Air Blank	0.000	08:32
Cal Check	0.100	08:33
Air Blank	0.000	08:33
Cal Check	0.100	08:34
Air Blank	0.000	08:34
Cal Check	0.100	08:35
Air Blank	0.000	08:36
Cal Check	0.099	08:36
Air Blank	0.000	08:37
Cal Check	0.099	08:38
Air Blank	0.000	08:38
Cal Check	0.099	08:39
Air Blank	0.000	08:39
Cal Check	0.100	08:40
Air Blank	0.000	08:41
Cal Check Stats		
Average	0.0996	
Std Dev	0.0005	
Rel Std Dev(%)	0.5184	

 16837  
 Operator's Signature

  
 Ted L. Pauley, President  
 GUTH LABORATORIES, INC.

**NIST Traceability:**  
 Testing was conducted using Cerilliant Reference Standard lot number FN04271602 whose values are traceable to NIST.  
 All balances are calibrated annually by an outside agency using NIST traceable weights.  
 Calibration verification is done prior to each use utilizing NIST traceable weights.

Certificate of Analysis - Wet Bath	
09-27-2018	.200
Date of Analysis	Labelled target value (g/210L)
17340	0.1968
Lot Number	test result (g/210L)
	
<b>GUTH LABORATORIES, INC.</b> 500 NORTH 67th STREET • HARRISBURG, PA 17111-4611 • TELEPHONE: 717-564-5470	
BOT Technician Name and Signature: <b>Josh Smith</b> <small>BRT Form 6.0</small>	



In accordance with BRT - 2.1.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

**CERTIFICATE OF ANALYSIS**

Certified Alcohol Reference Solution for Simulator

*REC'D  
08/25/18  
[Signature]*

Random Samples of Lot Number 17340 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on **October 10, 2017**, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain **0.2410%** (w/vol) ethyl alcohol. The expiration date for this lot number is **October 9, 2019** at 11:59 PM.

ALPHA INSTRUMENT  
Intoxilyzer - Alcohol Analyzer  
Model 8000  
09/27/2018  
SN 80-002591  
15:27

Test	g/210L	Time
Air Blank	0.000	15:27
Cal Check	0.196	15:28
Air Blank	0.000	15:29
Cal Check	0.196	15:29
Air Blank	0.000	15:30
Cal Check	0.197	15:31
Air Blank	0.000	15:31
Cal Check	0.197	15:32
Air Blank	0.000	15:33
Cal Check	0.197	15:33
Air Blank	0.000	15:34
Cal Check	0.197	15:35
Air Blank	0.000	15:35
Cal Check	0.197	15:36
Air Blank	0.000	15:36
Cal Check	0.197	15:37
Air Blank	0.000	15:38
Cal Check	0.197	15:38
Air Blank	0.000	15:39
Cal Check	0.197	15:40
Air Blank	0.000	15:40
Cal Check Stats		
Average	0.1968	
Std Dev	0.0004	
Rel Std Dev(%)	0.2142	

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of **0.200 g/210L +/- 3%**.

The alcohol and water used in this solution were free of test interfering substances.

*Ted L. Pauley*  
 Ted L. Pauley, President  
 GUTH LABORATORIES, INC.

*[Signature]* 16837  
 Operator's Signature

**NIST Traceability:**

Testing was conducted using Cerilliant Reference Standard lot number **FN08101505** whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.