



**STATE OF OKLAHOMA
BOARD OF TESTS FOR ALCOHOL AND DRUG INFLUENCE**

Post Office Box 36307

Oklahoma City, Oklahoma 73136-2307
Phone: (405) 425-2460 Fax: (405) 425-2490
www.bot.ok.gov

Dr. Jarrad Wagner, Ph.D. F-ABFT
Chairman


Joshua Smith
Director

ATTESTATION

I, the undersigned Joshua Smith (Director/Records Custodian), attest under oath pursuant to 12 O.S. §2902 (11)(a) this record was made, at or near the time of the occurrence of the matters set forth by or from information transmitted by a person having knowledge of those matters; was kept in the course of the regularly conducted business activity of the Board; and was made pursuant to the regularly conducted activity. The duplicate record provided is listed below:

- 1) The attached "Service Overview" is a true and accurate copy of maintenance performed on the Intoxilyzer 8000, serial number _____, in compliance with the agency's Maintenance Policy and Procedures.

This packet consists of _____ pages.

Signed 

Name of Position: Director/Records Custodian

Date of Attestation:

Service Overview

Board of Tests for Alcohol and Drug Influence
Enhancing public safety by ensuring the accuracy and scientific reliability
of blood and breath testing



3600 N. Martin Luther King Bldg #9
Oklahoma City, OK 73111
405-425-2460

BENCH CHECK DATE: 06-17-2021

SERIAL: 80-006119

DOCUMENTATION WITHIN SERVICE PACKET:

- BOT Certificate of Calibration and Operation
- CMI Certificate of Calibration 06-11-2021
- Bench Check
- Bench Check Technician's Report
- BOT Dry Gas Certificate of Analysis
- CMI Service Evaluation Form
- CMI Work Order
- Mock Subject Test
- BOT Certificates of Analysis on Certified Solutions (4)



STATE OF OKLAHOMA
BOARD OF TESTS FOR ALCOHOL AND DRUG INFLUENCE

Administrative Office at:
 Board of Tests for Alcohol and Drug Influence
 Post Office Box 36307
 Oklahoma City, Oklahoma 73136-2307

Certificate of Calibration and Operation

This is to certify that the calibration of **INTOXILYZER 8000**, serial number 80-006119, manufactured by CMI Inc., a subsidiary of MPD, Inc. of Owensboro, Kentucky, was tested and found to be in compliance with National Highway Traffic Safety Administration Standard for Devices to Measure Breath Alcohol (F.R., No. 179 48705-48710 Sept. 17, 1993) and with International Recommendation OIML R 126 Edition 1998 (E). Calibration solutions are traceable to NIST standard material 1828.

In addition the operational procedures and functions of this Intoxilyzer have also been tested and found to be in compliance with the Oklahoma Board of Tests for Alcohol and Drug Influence - Rules and Regulations OAC Title 40: 25-1-2 and 30-1-3 and is hereby certified for use as an evidential breath testing device within this state.

CERTIFICATION TYPE	DATE
Manufacturer Calibration	12-05-13
Board of Tests Bench Check	12-13-13
Board of Tests Bench Check	10-07-15
Board of Tests Bench Check	06-12-17
Board of Tests Bench Check	06-06-19
Manufacturer Calibration	06-11-21
Board of Tests Bench Check	06-17-21



Presentation of this form certifies that the Intoxilyzer, SN: 80-006119, functioned properly at the time of the breath test and hereby certifies the breath test result as valid.

Date:

Re: Request for Log of Test on Intoxilyzer 8000

Name:

Dear Sir:

The Log of Test information from a breath test conducted on a Intoxilyzer 8000 is printed in Section 2 of the Affidavit and is no longer retained as a separate form as with the Intoxilyzer 5000. The 8000 uses a nitrogen/ethanol dry gas for the external control test. The dry gas cylinder has the capacity to perform approximately 325 tests and does not require maintenance until its expiration date or can no longer provide the required pressure to perform a control test. The cylinder has an expiration date of two years from date filled at the manufacturer and is programmed in the 8000 upon installation, both dates are printed in Section 2 of the Affidavit. The Intoxilyzer is programmed to disable itself when the date of expiration is reached or the pressure monitor indicates 25 lbs psi.

Due to the reliability and stability of dry gas, maintenance on the 8000 is not required every 30 days or 25 tests, therefore maintenance is no longer performed by officers in the field. The Board of Tests for Alcohol and Drug Influence certifies each Intoxilyzer 8000 for field use by performing a bench check. The bench check is designed to check the operation and procedures programmed in the 8000 to ensure it is functioning properly for use in Oklahoma. A bench check is performed every time a new dry gas cylinder is installed or the instrument has returned from the manufacturer for repair. Once the instrument passes the bench check, all that is required to set it up for field use is to plug it in and turn it on and does not require a permit to set up. The Board of Tests has the ability to monitor each instrument once it is set up in the field.

Each Intoxilyzer has a database of valid permit numbers that it checks prior to allowing a breath test to be performed. The database is updated on a regular basis, if a permit number is invalid that officer will not be able to conduct a breath test on the 8000. If the 8000 prints an affidavit the breath test operator listed in Section 2 had a valid permit at the time of the test and the breath test is valid.

If you have any further questions please feel free to call me.

Sincerely,



J. Robert Blakeburn (OBA11059)
State Director of Tests for Alcohol
and Drug Influence

Certificate of Calibration

This is to certify the calibration of **Intoxilyzer**® serial number 80-006119, manufactured by CMI Inc., a subsidiary of MPD, Inc. of Owensboro, Kentucky, was tested and found to conform to the National Highway Traffic Safety Administration (NHTSA) Standard for Devices to Measure Breath Alcohol (Federal Register, Vol.58, No.179, pp 48705-48710, Sept. 17, 1993) for accuracy and precision. Reference materials are traceable through the National Institute of Standards and Technology (NIST) to the International System of Units (SI).

Date June 11, 2021 Signed Alice Soler

Technician



316 East 9th Street
Owensboro, KY 42303
USA

Part No. 650517 Rev.A

STATE OF OKLAHOMA - BOARD OF TESTS FOR ALCOHOL AND DRUG INFLUENCE CMI INTOXILYZER BENCH CHECK PROCEDURE REPORT

BENCH CHECK DATE 06/17/2021	TIME PROCEDURE BEGAN 09:10:4	INSTRUMENT LOCATION 80-006119
INSTRUMENT TYPE Intoxilyzer	INSTRUMENT MODEL I-8000	INSTRUMENT SERIAL NUMBER 80-006119

TEST RESULTS

Diagnostics

PASS

Mouth Alcohol Test

PASS

RFI Test

PASS

Abort Test

PASS

Improper Sample Test

PASS

Interferent Detect Test

PASS

No Sample Given Test

PASS

Insufficient Sample Test

PASS

Air Blank Contamination Test

PASS

Range Exceeded Test

PASS


Duplicate Breath Sampling Results

Value	Test 1	Test 2	Control Test
.02	0.019	0.018	0.019
.04	0.037	0.037	0.038
.10	0.098	0.097	0.098
.20	0.199	0.196	0.197

PASS

CERTIFYING TECHNICIAN

I swear under penalty of perjury that in regards to the above listed instrument, I have complied with the Intoxilyzer Bench Checking Procedure approved by the State of Oklahoma.

SIGNATURE  23020	DATE 6/17/2021
NAME PAPE, CHRISTOPHER	PERMIT # 0000023020



3600 N. Martin Luther King Bldg #9
 Oklahoma City, OK 73111
 405-425-2460

BENCH CHECK TECHNICIAN'S REPORT

Date: 06/17/2021

Start Time: 09:05

End Time: 10:35

INSTRUMENT

Intoxilyzer Model	Serial #
8000	80-006119

GAS CANISTER

LOT #	EXP Date
08121080A1-069	05/05/2023

REFERENCE


Simulator Model			
Guth 2100	Guth 2100	Guth 2100	Guth 2100
Serial #			
DR2834	DR3700	DR2455	DR3470
Concentration			
.02	.04	.10	.20
LOT #			
20070	20060	20190	20160
Manufactured Date			
02/13/2020	02/10/2020	04/06/2020	03/18/2020
Expiration Date			
02/13/2022	02/10/2022	04/06/2022	03/18/2022
Solution Commission Date			
6/3/2021	6/3/2021	6/3/2021	6/11/2021

REASON FOR BENCH CHECK

- POST REPAIR
 CYLINDER REPLACEMENT
 TROUBLESHOOTING
 ROUTINE MAINTENANCE


COMMENTS

Replaced Pump and Exhaust Block at BOT. CMI found leak in cell block. Replaced diode and O-Rings.

 23020
 Technician Signature / Permit #

Christopher Pape #23020
 Printed Name

Certificate of Analysis – Dry Gas	
5/14/2021	0.080
Date of Analysis	Labelled target value (g/210L)
069	0.081
Cylinder #	Average test result
Christopher Pape <i>[Signature]</i> 23020	
BOT Technician Name and Signature	

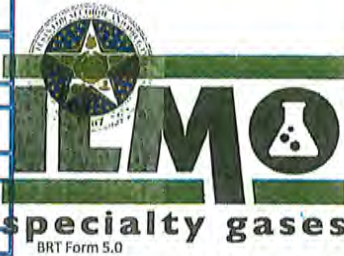

8/16

ALPHA INSTRUMENT
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-002591
05/14/2021 11:54

In accordance with BOT Policy and Procedure Statement 7 Eastgate Dr., P.O. Box 790 • Jacksonville, IL 62651-0790
referenced dry gas cylinder is suitable for use as an external reference with the Intoxilyzer 8000
217-245-2183 • Fax: 217-243-7634 • www.ilmoproducts.com

Test	g/210L	Time
Air Blank	0.000	11:54
Cal Check	0.081	11:55
Air Blank	0.000	11:55
Cal Check	0.081	11:56
Air Blank	0.000	11:56
Cal Check	0.081	11:56
Air Blank	0.000	11:57
Cal Check	0.081	11:57
Air Blank	0.000	11:58
Cal Check	0.081	11:58
Air Blank	0.000	11:59
Cal Check	0.081	11:59
Air Blank	0.000	11:59
Cal Check	0.081	12:00
Air Blank	0.000	12:00
Cal Check	0.081	12:01
Air Blank	0.000	12:01
Cal Check	0.081	12:01
Air Blank	0.000	12:02
Cal Check	0.081	12:02
Air Blank	0.000	12:02
Cal Check	0.081	12:03
Cal Check Stats		
Average	0.0810	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Certificate of Analysis

*RCV'D
4/30/2021
CP*

Certificate ID: 13813
Part #: BAC105L080T
Cylinder Size: 105L
Lot Number: 08121080A1
Expiration: 5/5/2023

0.080 BAC (For the calibration of instruments used to determine breath alcohol concentration)

Contents: 105 Liters @ 1000 psig 70°F (21°C)

Component:	Reported Concentration:	Analytical Accuracy (U, k=2):	Analytical Method:
Ethanol	208 ppm	+/-0.002 BAC(G/210L) [5.2 ppm]	NDIR
Nitrogen	Balance		

Distributed by:

CMI Inc.
316 East Ninth St
Owensboro, KY
Phone 866-835-0
www.alcoholtest

[Signature]
Operator's Signature

*Traceable to:
Certified Reference Material - 262.4 µmol/mol
Ethanol in Nitrogen - Serial No. GN0015026 Lot No. 050319E11

Store in dry area, away from sources of heat, ignition and direct sunlight. Do not allow storage area to exceed 52 °C (125 °F).

[Signature]
Specialty Gas Lab Tech
[Signature]

04-22-2021
Issuance Date



The calibration results within this certificate were obtained using equipment and standards capable of producing analytical results traceable to NIST, and apply only to the items contained on this certificate. ILMO Products Company makes no warranty or representation as to the suitability of the use of any information provided for any particular purpose. The information use is at the sole discretion and risk of the user. Liability shall be limited to established replacement cost of this material or service.

Service Evaluation Form

**This form MUST be completed and enclosed with instrument to be serviced.
Failure to complete and return this form may cause delays in service.**

(Note: please ship items in their original shipping container(s) or a similar protective box.)

1. Contact information: Customer Number **731362** (contact Customer Service)
Name: **Board of Tests** Phone: **(405) 425 2460**
Fax: **(405) 425 2490** Email: **christopher.pape@bot.ok.gov**

2. Bill to Address: **Board of Tests** Ship to Address: **Board of Tests**
3600 N ML King, Bldg 9 **3600 N ML King, Bldg 9**
OKC, OK 73111 **OKC, OK 73111**

3. Serial Number: **80-006119** Instrument Model: **Intoxilyzer 500 / 8000**

4. Detailed Description of Problem:
Unit came in with multiple purge fails. Replaced Exhaust block assembly and pump. Unit still does not purge. 3µm and 9µm DVM values drop with just air. 3µm fails snap test. Possible issue with source. Please replace if necessary.

Hazardous Material Warning! - DO NOT return gas cylinders with instrument!

I Authorize Repairs Up To: All \$250 \$500 \$750 Other \$ _____
Purchase Order Number (attach a copy of P.O. if applicable) _____

Authorized By:

Ship to:

Chris Pape

Breath Testing Admin

Name (Please Print)

Title

CMI, Inc

Signature

03/10/2021

Date

Attn: Service Dept.

316 East Ninth Street

Owensboro, KY 42303

Call: 405-425-2460 or email

No, please send estimate before repairs are made.

Note: An estimate will be faxed before performing any repairs and may cause delays in service.
An evaluation fee (\$79.00 or actual costs) will apply to estimates that are not repaired.



SERVICE WORK ORDER

DATE: 3/17/2021

316 E 9th Street / Owensboro KY 42303 / USA
 Phone: 866-835-0690 Fax: 270-685-6268

405836

Bill To:
 Oklahoma Board Of Tests For Alcohol And Drug Infl
 Po Box 36307
 3600 N MI King Blvd Blg 9
 Oklahoma City, OK 73111
 USA
 Customer #: 731110

Ship To:
 Oklahoma Board Of Tests DNU
 Po Box 36307
 3600 N MI King Blvd Blg 9
 Oklahoma City OK 73111
 USA
 Fax: 405-425-2324

MODEL #: 0024800K

Serial Number: 80-006119

BILL CODE: Out of Warranty

EXTRA PARTS RCVD:

KB,BH,BATTERY COVER,GAS SHELF W/GAS REG GR-2696

DESCRIPTION OF PROBLEM

UNIT CAME IN WITH MULTIPLE PURGE FAILS.REPLACED EXHAUST BLOCK ASS AND PUMP. UNIT STILL DOES NOT PURGE.3*M AND 9*M DVM VALUES DROP WITH KUST AIR. 3*M FAILS SNAP TEST. POSSIBLE ISSUE WITH SOURCE. PLEASE REPLACE IF NECESSARY.

WORK PERFORMED:

- Issues with DVM's and purge fail were caused by a leak in the cell
- Repaired leak in cell
- Source was OK
- Filter / dirty
- Connector / damaged
- O-rings / cracked
- Replaced parts listed
- Calibrated and final tested
- Records deleted per Josh Smith
- Reinstalled CR25 on system board

PARTS USED

Seq. No.	Part	Description	Quantity
50	470202	FILTER,FOAM,1.85x2.20	1.00 EA
60	471201	O-RING,BUNA-N,-008,3/16inx5/16	1.00 EA
70	320383	HSG,SKT,CONN,04CKT.156CC,LKG	1.00 EA
80	650517	CERTIFICATE OF CALIBRATION	2.00 EA
90	441169	COVER DUST,5/8in x 1/2in	1.00 EA
100	470145	CAP,PLASTIC,.25IDx.50LG,RED	3.00 EA
110	470154	CAP,PLSTC,.406IDx.438-.562,RED	1.00 EA
120	470218	SEAL,TAMPER EVIDENT,SERVICE	1.00 EA
140	923002	DIODE,SMD,1N4148,SOT-23	1.00 EA
150	402565	O-RING,NEOPRENE,.301IDx.06THK	1.00 EA

LABOR / TESTING

Misc Code	Description	Hours
LABR	Service Repair Labor	
LABR	Service Repair Labor	
LFT	Service - Cal / Final Test	1.00

Technician Name: Leanna Shelnut

SRV4058360001



OFFICER'S AFFIDAVIT AND NOTICE OF REVOCAION/DISQUALIFICATION

11/16

Section 1

ARREST DATE 06/17/2021		ARREST TIME 1000		COUNTY # 55	CITY #	CITATION #			
ARREST LOCATION BOT				CITY		COUNTY OKLAHOMA			
SUBJECT NAME NORTH, GAYLON LEVERNE				DATE OF BIRTH 08/09/1961		SEX M	RACE W	HEIGHT 510	WEIGHT 165
ADDRESS 3600 MARTIN LUTHER KING A			CITY OKLAHOMA CITY			STATE OK	ZIP CODE 73133		
DRIVER LICENSE # T083454871				EXPIRATION DATE 06/30/2019		STATE OK	CLASS A	RESTRICTIONS	ENDORSEMENTS M
VEHICLE MAKE MOCK		MODEL MOCK		TAG # MOCK		STATE OK	CMV N	PLACARD N	

On the above date, time, and location, the above named person was arrested, and I had reasonable grounds to believe the person was driving or in actual physical control of a motor vehicle upon a public road, highway, street, turnpike, public parking lot, or other public place, or upon a private road, street, alley or lane which provides access to one or more single or multi-family dwelling within this state while under the influence of alcohol and/or other intoxicating substances as prohibited by law.

(Describe driving behavior or circumstances):

MOCK SUBJECT TEST

Describe person's condition (odor, actions, etc.):

POST REPAIR MAINTENANCE, INSTALLED NEW CYLINDER

THE PERSON WAS INFORMED OF THE IMPLIED CONSENT TEST REQUEST

BREATH-ALCOHOL ANALYSIS RECORD, REPORT OF THE PERSON NAMED IN SECTION 1 ABOVE, and LOG OF TEST AND MAINTENANCE RECORD.

Section 2

EQUIPMENT I-8000		SERIAL NUMBER 80-006119	SPECIALIST BOARD OF TESTS																																					
STANDARD Dry		TARGET VALUE 0.080	PERMIT NUMBER 23020																																					
MANUFACTURER ILMO		LOT # 08121080A1	DATE CYLINDER INSTALLED 06/17/2021	DATE CYLINDER EXPIRES 05/05/2023																																				
OBSERVATION START 1010	TEST DATE 06/17/2021	MOUTHPIECE G	<p style="text-align: center;">A 15-minute (or greater) deprivation/observation period was observed prior to and continuing to the time of test administration.</p> <p style="text-align: center;">I administered said Breath-Alcohol Test in compliance with the applicable operating procedure of the Board of Tests.</p> <p style="text-align: center;"><i>Christopher Pape</i> SIGNATURE OF OPERATOR</p>																																					
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.00</td><td>10:30</td></tr> <tr><td>Subject Test</td><td>0.00</td><td>10:31</td></tr> <tr><td>Breath Volume</td><td>1.820 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:31</td></tr> <tr><td>Wait</td><td></td><td>10:33</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:33</td></tr> <tr><td>Subject Test</td><td>0.00</td><td>10:34</td></tr> <tr><td>Breath Volume</td><td>1.812 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:34</td></tr> <tr><td>Cal Check</td><td>0.07</td><td>10:35</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:35</td></tr> </tbody> </table>					Test	g/210L	Time	Air Blank	0.00	10:30	Subject Test	0.00	10:31	Breath Volume	1.820 LITERS		Air Blank	0.00	10:31	Wait		10:33	Air Blank	0.00	10:33	Subject Test	0.00	10:34	Breath Volume	1.812 LITERS		Air Blank	0.00	10:34	Cal Check	0.07	10:35	Air Blank	0.00	10:35
Test	g/210L	Time																																						
Air Blank	0.00	10:30																																						
Subject Test	0.00	10:31																																						
Breath Volume	1.820 LITERS																																							
Air Blank	0.00	10:31																																						
Wait		10:33																																						
Air Blank	0.00	10:33																																						
Subject Test	0.00	10:34																																						
Breath Volume	1.812 LITERS																																							
Air Blank	0.00	10:34																																						
Cal Check	0.07	10:35																																						
Air Blank	0.00	10:35																																						
RESULT TABLE			NAME PAPE, CHRISTOPHER																																					
			BADGE # 000000484	PERMIT # 0000023020																																				
			AGENCY BOARD OF TESTS																																					

EFFECTIVE THIRTY (30) DAYS FROM DATE SERVED. Notice of Revocation is given that your driver's license is revoked or denied for a period of one hundred eighty (180) days or more, if you refused or failed the state's test(s). In addition, your commercial driving privilege in this state will be disqualified if you refused or failed the state's test(s) (operating a CMV or CDL holder) OR a test result of .04 or more while operating a commercial motor vehicle. You may appeal any Departmental action against your driver license as a result of this arrest by filing a petition in the District Court of the County in which you were arrested. Your petition must be filed within thirty (30) days of the date listed below. You may be eligible to participate in the Impaired Driver Accountability Program (IDAP) administered by the Department of Public Safety (DPS). Completion of IDAP may prevent a revocation as a result of this arrest from appearing on your driving record. Participation in IDAP may reduce the amount of fees you will be required to pay to the State. You must request IDAP within thirty (30) days of the date listed below. Mail the request for IDAP to the Department of Public Safety at P.O. Box 11415, Oklahoma City, OK 73136.

SERVING OF NOTICE: I personally hand delivered a copy of the above containing the Notice of Revocation and the Notice of Department Impaired Driving Accountability Program to the person named in Section 1 above.

Date served: **06/17/2021** Signature of officer: _____ Badge #: _____

In accordance with Title 12 O.S. Section 426, "I state under penalty of perjury under the laws of Oklahoma that the foregoing is true and correct." Section 4

Date: **06/17/2021** Place (location when signed): _____ Signature of arresting officer: _____

NAME PAPE, CHRISTOPHER		AGENCY BOARD OF TESTS	
BADGE 000000484	AGENCY ADDRESS INTER-AGENCY	ZIP CODE 00000	PHONE 4054252460

OTHER WITNESSES:

Section 5

1	NAME	TITLE	ADDRESS	PHONE
2	NAME	TITLE	ADDRESS	PHONE

No Temporary License Issued:
Test Below Legal Limit

OFFICER/DPS COPY
BOT Form AFF01 03/2020

OFFICER'S AFFIDAVIT AND NOTICE OF REVOCATION/DISQUALIFICATION

12/16

Section 1

ARREST DATE 06/17/2021		ARREST TIME 1000		COUNTY # 55	CITY #	CITATION #		
ARREST LOCATION BOT				CITY	COUNTY OKLAHOMA			
SUBJECT NAME NORTH, GAYLON LEVERNE				DATE OF BIRTH 08/09/1961	SEX M	RACE W	HEIGHT 510	WEIGHT 165
ADDRESS 3600 MARTIN LUTHER KING A			CITY OKLAHOMA CITY		STATE OK	ZIP CODE 73133		
DRIVER LICENSE # T083454871			EXPIRATION DATE 06/30/2019	STATE OK	CLASS A	RESTRICTIONS	ENDORSEMENTS M	
VEHICLE MAKE MOCK		MODEL MOCK	TAG # MOCK		STATE OK	CMV N	PLACARD N	

On the above date, time, and location, the above named person was arrested, and I had reasonable grounds to believe the person was driving or in actual physical control of a motor vehicle upon a public road, highway, street, turnpike, public parking lot, or other public place, or upon a private road, street, alley or lane which provides access to one or more single or multi-family dwelling within this state while under the influence of alcohol and/or other intoxicating substances as prohibited by law.

(Describe driving behavior or circumstances):

MOCK SUBJECT TEST

Describe person's condition (odor, actions, etc.):

POST REPAIR MAINTENANCE, INSTALLED NEW CYLINDER

THE PERSON WAS INFORMED OF THE IMPLIED CONSENT TEST REQUEST

BREATH-ALCOHOL ANALYSIS RECORD, REPORT OF THE PERSON NAMED IN SECTION 1 ABOVE, and LOG OF TEST AND MAINTENANCE RECORD.

Section 2

EQUIPMENT I-8000		SERIAL NUMBER 80-006119	SPECIALIST BOARD OF TESTS																																					
STANDARD Dry		TARGET VALUE 0.080	PERMIT NUMBER 23020																																					
MANUFACTURER ILMO		LOT # 08121080A1	DATE CYLINDER INSTALLED 06/17/2021	DATE CYLINDER EXPIRES 05/05/2023																																				
OBSERVATION START 1010	TEST DATE 06/17/2021	MOUTHPIECE G	<p style="text-align: center;">A 15-minute (or greater) deprivation/observation period was observed prior to and continuing to the time of test administration.</p> <p style="text-align: center;">I administered said Breath-Alcohol Test in compliance with the applicable operating procedure of the Board of Tests.</p> <p style="text-align: center;"><i>Christopher Pape</i> SIGNATURE OF OPERATOR</p>																																					
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.00</td><td>10:30</td></tr> <tr><td>Subject Test</td><td>0.00</td><td>10:31</td></tr> <tr><td> Breath Volume</td><td>1.820 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:31</td></tr> <tr><td>Wait</td><td></td><td>10:33</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:33</td></tr> <tr><td>Subject Test</td><td>0.00</td><td>10:34</td></tr> <tr><td> Breath Volume</td><td>1.812 LITERS</td><td></td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:34</td></tr> <tr><td>Cal Check</td><td>0.07</td><td>10:35</td></tr> <tr><td>Air Blank</td><td>0.00</td><td>10:35</td></tr> </tbody> </table>					Test	g/210L	Time	Air Blank	0.00	10:30	Subject Test	0.00	10:31	Breath Volume	1.820 LITERS		Air Blank	0.00	10:31	Wait		10:33	Air Blank	0.00	10:33	Subject Test	0.00	10:34	Breath Volume	1.812 LITERS		Air Blank	0.00	10:34	Cal Check	0.07	10:35	Air Blank	0.00	10:35
Test	g/210L	Time																																						
Air Blank	0.00	10:30																																						
Subject Test	0.00	10:31																																						
Breath Volume	1.820 LITERS																																							
Air Blank	0.00	10:31																																						
Wait		10:33																																						
Air Blank	0.00	10:33																																						
Subject Test	0.00	10:34																																						
Breath Volume	1.812 LITERS																																							
Air Blank	0.00	10:34																																						
Cal Check	0.07	10:35																																						
Air Blank	0.00	10:35																																						
RESULT TABLE			NAME PAPE, CHRISTOPHER																																					
			BADGE # 0000000484	PERMIT # 0000023020																																				
			AGENCY BOARD OF TESTS																																					

EFFECTIVE THIRTY (30) DAYS FROM DATE SERVED. Notice of Revocation is given that your driver's license is revoked or denied for a period of one hundred eighty (180) days or more, if you refused or failed the state's test(s). In addition, your commercial driving privilege in this state will be disqualified if you refused or failed the state's test(s) (operating a CMV or CDL holder) OR a test result of .04 or more while operating a commercial motor vehicle. You may appeal any Departmental action against your driver license as a result of this arrest by filing a petition in the District Court of the County in which you were arrested. Your petition must be filed within thirty (30) days of the date listed below.

Section 3

You may be eligible to participate in the Impaired Driver Accountability Program (IDAP) administered by the Department of Public Safety (DPS). Completion of IDAP may prevent a revocation as a result of this arrest from appearing on your driving record. Participation in IDAP may reduce the amount of fees you will be required to pay to the State. You must request IDAP within thirty (30) days of the date listed below. Mail the request for IDAP to the Department of Public Safety at P.O. Box 11415, Oklahoma City, OK 73136.

SERVING OF NOTICE: I personally hand delivered a copy of the above containing the Notice of Revocation and the Notice of Department Impaired Driving Accountability Program to the person named in Section 1 above.

Date served: **06/17/2021** Signature of officer: _____ Badge #: _____

In accordance with Title 12 O.S. Section 426, "I state under penalty of perjury under the laws of Oklahoma that the foregoing is true and correct."

Section 4

Date: **06/17/2021** Place (location when signed): _____ Signature of arresting officer: _____

NAME PAPE, CHRISTOPHER		AGENCY BOARD OF TESTS	
BADGE 0000000484	AGENCY ADDRESS INTER-AGENCY	ZIP CODE 00000	PHONE 4054252460

No Temporary License Issued:
Test Below Legal Limit

ARRESTEE'S COPY
BOT Form AFF02 03/2020

Certificate of Analysis - Wet Bath	
8/11/2020	0.020
Date of Analysis	Labelled target value (g/210L)
20070	0.020
Lot Number	Average test result (g/210L)
christopher Pipe	
BOT Technician Name and Signature	



GUTH LABORATORIES, INC.

155 NORTH 3RD STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

BRT Form 6.0

In accordance with BRT - 2.2.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer B000.

CERTIFICATE OF ANALYSIS

ACV'D
6/1/2020
CP

ALPHA INSTRUMENT 2
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-004923
08/11/2020 09:42

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number **20070** of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on **February 17, 2020**, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain **0.0242%** (w/vol) ethyl alcohol. The expiration date for this lot number is **February 13, 2022** at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of **0.020 g/210L +/- 3%**.

The alcohol and water used in this solution were free of test interfering substances.

Test	g/210L	Time
Air Blank	0.000	09:42
Cal Check	0.020	09:43
Air Blank	0.000	09:43
Cal Check	0.020	09:44
Air Blank	0.000	09:45
Cal Check	0.020	09:45
Air Blank	0.000	09:46
Cal Check	0.020	09:47
Air Blank	0.000	09:47
Cal Check	0.021	09:48
Air Blank	0.000	09:48
Cal Check	0.020	09:49
Air Blank	0.000	09:49
Cal Check	0.020	09:50
Air Blank	0.000	09:51
Cal Check	0.020	09:51
Air Blank	0.000	09:52
Cal Check	0.020	09:53
Air Blank	0.000	09:53
Cal Check	0.019	09:54
Air Blank	0.000	09:54
Cal Check Stats		
Average	0.0200	
Std Dev	0.0004	
Rel Std Dev(%)	2.3569	

Christopher Pipe
Operator's Signature

Ted L. Pauley
Ted L. Pauley, President
GUTH LABORATORIES, INC.

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN08031603 whose values are traceable to NIST. All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.



Certificate of Analysis - Wet Bath	
7/22/2020	0.040
Date of Analysis	Labelled target value (g/210L)
20060	0.040
Lot Number	Average test result (g/210L)
Christopher Pauley	
BRT Form 6.0	

In accordance with BRT -- 2.2.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

GUTH LABORATORIES, INC.
 600 NORTH 60th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

RCV'D
6/1/20
CP

Random Samples of Lot Number 20060 ✓ of

Alcohol Reference Solution for Simulator were analyzed by gas chromatography on February 11, 2020, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.0483% (w/vol) ethyl alcohol. The expiration date for this lot number is February 10, 2022 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.040 g/210L +/- 3% ✓

The alcohol and water used in this solution were free of test interfering substances.

ALPHA UNIT SUB
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-003400
 07/22/2020 14:57

Test	g/210L	Time
Air Blank	0.000	14:57
Cal Check	0.040	14:58
Air Blank	0.000	14:59
Cal Check	0.039	14:59
Air Blank	0.000	15:00
Cal Check	0.039	15:01
Air Blank	0.000	15:01
Cal Check	0.039	15:02
Air Blank	0.000	15:02
Cal Check	0.039	15:03
Air Blank	0.000	15:04
Cal Check	0.039	15:04
Air Blank	0.000	15:05
Cal Check	0.040	15:06
Air Blank	0.000	15:06
Cal Check	0.040	15:07
Air Blank	0.000	15:07
Cal Check	0.040	15:08
Air Blank	0.000	15:09
Cal Check	0.040	15:09
Air Blank	0.000	15:10
Cal Check Stats		
Average	0.0395	
Std Dev	0.0005	
Rel Std Dev(%)	1.3342	

Ted L. Pauley, President
 GUTH LABORATORIES, INC.

Operator's Signature

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN12181501 whose values are traceable to NIST.
 All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.



Date of Analysis	06/16/20	Labelled target value (g/210L)	.100
Lot Number	20190	Average test result (g/210L)	.098
BOT Technician Name and Signature: <i>Josh Smith</i>			

GUTH LABORATORIES, INC.
 1001 N. 15th St., P.O. Box 111, Roseburg, PA 17111-4511 • TELEPHONE: 717-564-5470
 BRT Form 6.0

In accordance with BRT - 2.2.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

*Rec'd
06/11/2020*

CERTIFICATE OF ANALYSIS

ALPHA INSTRUMENT
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-002591
 06/16/2020 16:18

Certified Alcohol Reference Solution for Simulator

Test	g/210L	Time
Air Blank	0.000	16:18
Cal Check	0.099	16:19
Air Blank	0.000	16:20
Cal Check	0.098	16:20
Air Blank	0.000	16:21
Cal Check	0.097	16:22
Air Blank	0.000	16:22
Cal Check	0.098	16:23
Air Blank	0.000	16:24
Cal Check	0.098	16:24
Air Blank	0.000	16:25
Cal Check	0.098	16:26
Air Blank	0.000	16:26
Cal Check	0.098	16:27
Air Blank	0.000	16:27
Cal Check	0.097	16:28
Air Blank	0.000	16:29
Cal Check	0.098	16:29
Air Blank	0.000	16:30
Cal Check	0.098	16:31
Air Blank	0.000	16:31
Cal Check Stats		
Average	0.0979	
Std Dev	0.0005	
Rel Std Dev(%)	0.5798	

Random Samples of Lot Number 20190 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on April 8, 2020, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1206% (w/vol) ethyl alcohol. The expiration date for this lot number is April 6, 2022 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

[Signature]
 Operator's Signature 16037

[Signature]
 Ted L. Pauley, President
 GUTH LABORATORIES, INC.

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN02271802 whose values are traceable to NIST. All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.



Certificate of Analysis - Wet Bath	
07/07/2020	0.200
Date of Analysis	Labelled 1001 value (g/210L)
20160	0.197
Lot Number	Average Test Result (g/210L)
Christopher Pauley	2.5030
BOT Technician Name and Signature	

GUTH LABORATORIES, INC.
 590 NORTH 6TH STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

In accordance with BRT - 2.2.0, Maintenance, the above referenced simulator solution is suitable for use as an external reference in maintenance of the Intoxilyzer 8000.

CERTIFICATE OF ANALYSIS

*Rec'd
05/2020
CP*

Certified Alcohol Reference Solution for Simulator

LP4R UNIT SUB
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-003400
 7/07/2020 15:25

Test	g/210L	Time
1r Blank	0.000	15:26
3l Check	0.196	15:26
1r Blank	0.000	15:27
3l Check	0.196	15:28
1r Blank	0.000	15:28
3l Check	0.197	15:29
1r Blank	0.000	15:29
3l Check	0.196	15:30
1r Blank	0.000	15:31
3l Check	0.198	15:31
1r Blank	0.000	15:32
3l Check	0.198	15:33
1r Blank	0.000	15:33
3l Check	0.197	15:34
1r Blank	0.000	15:35
3l Check	0.198	15:35
1r Blank	0.000	15:36
3l Check	0.198	15:37
1r Blank	0.000	15:37
3l Check	0.197	15:38
1r Blank	0.000	15:38
3l Check Stats		
Average	0.1971	
Std Dev	0.0008	
Rel Std Dev(%)	0.4442	

Random Samples of Lot Number **20160** of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on March 20, 2020, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain **0.2427%** (w/vol) ethyl alcohol. The expiration date for this lot number is **March 18, 2022** at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of **0.200 g/210L +/- 3%**.

The alcohol and water used in this solution were free of test interfering substances.

[Signature]
 Operator's Signature

[Signature]
 Ted L. Pauley, President
 GUTH LABORATORIES, INC.

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number **FN08101505** whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.